


Ecogas - Weekly shift report

Mapse Barroso Ferreira Filho

Ecogas meeting - 21.April.2021



Report: 15/April

- HF measurements ongoing: Only CMS-GT-2-0 ON at 9.2 kV;
- Dew point at $\sim 5.51\text{ }^{\circ}\text{C}$ -> Adjusted back to $\sim 4\text{ }^{\circ}\text{C}$



Report: 19/April


- HF measurements ongoing: Only CMS-GT-2-0 ON at 11 kV;
- Dew point very high during the measurements

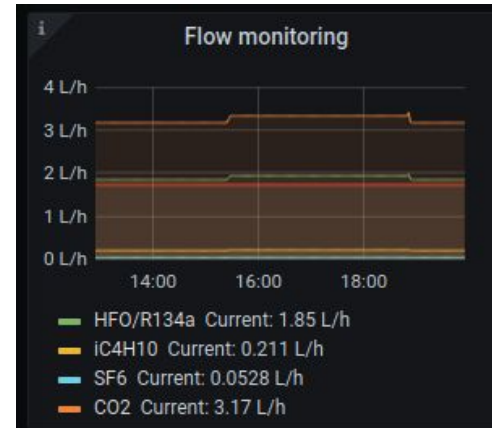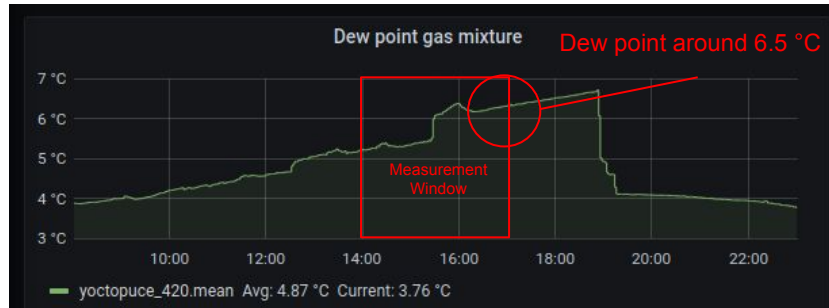

A slight change
in the flow

Report: 20/April

- Dew point was ~ 2 in the early morning. You can see the profile during the last night:

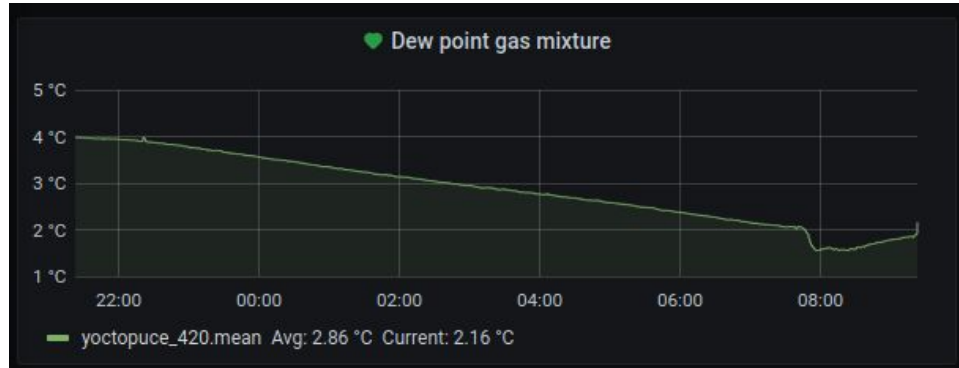

- I adjusted the dry mixture to 7.2 l/h and the Dew point was back to the acceptable values $\pm 4^{\circ}\text{C}$

Conclusions

- System seems behaving well
- Major issue was the high dew point and the gas flow variation at 19 of April.