
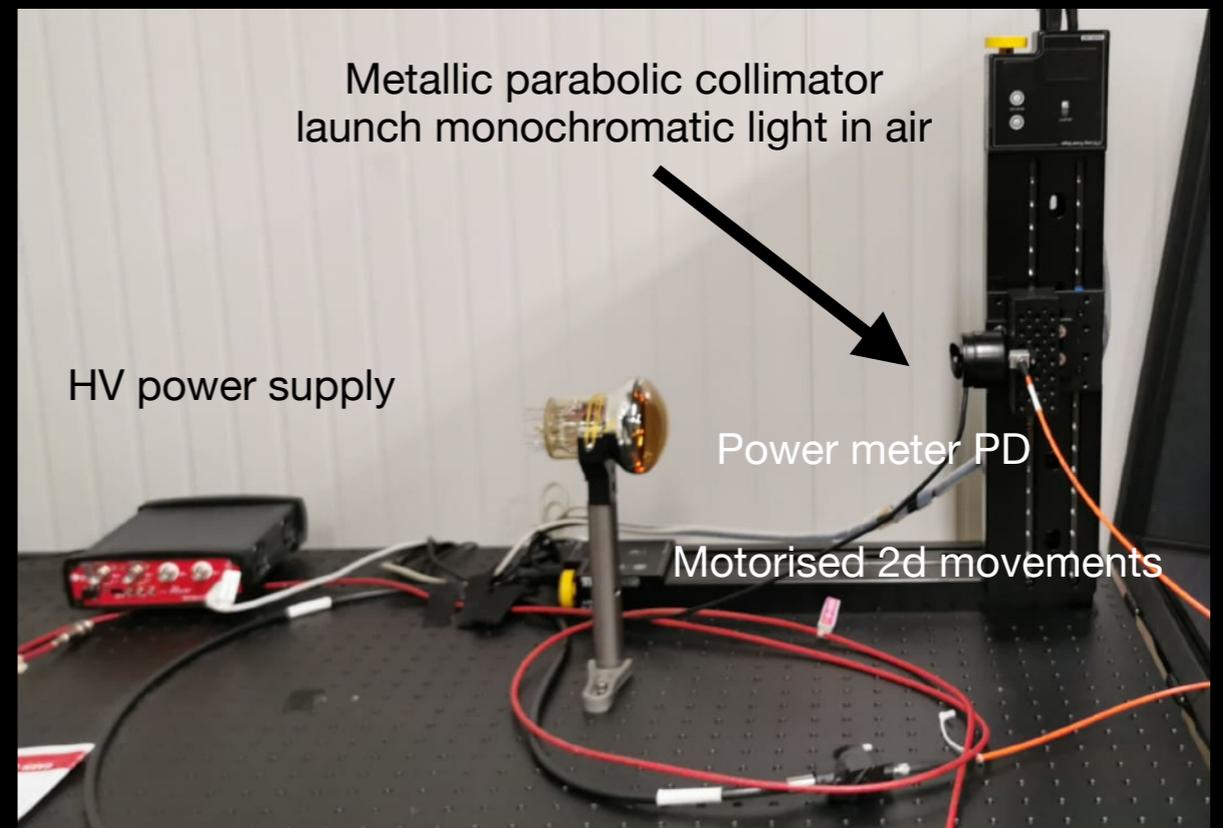


New measurements on an improved 3" Hamamatsu photomultiplier for the KM3NeT Neutrino Telescope

*Andreino Simonelli
INFN-Napoli
on behalf of KM3NeT
collaboration*




- Describe the new setup for Quantum Efficiency at INFN-Capacity lab in Caserta
- Show the QE measurements and compare the OLD R12199 (cfr. 2018 *JINST* **13** P05035) to the NEW R14374 PMTs
- Describe the special R14374 UBA increased QE PMT under test for possible future improvements
- Compare the time characteristics of a 500 set of new R14374 PMT using the Dark box apparatus to the old 3" PMT
- Conclusions

Experimental apparatus at CAPACITY lab of Caserta - INFN

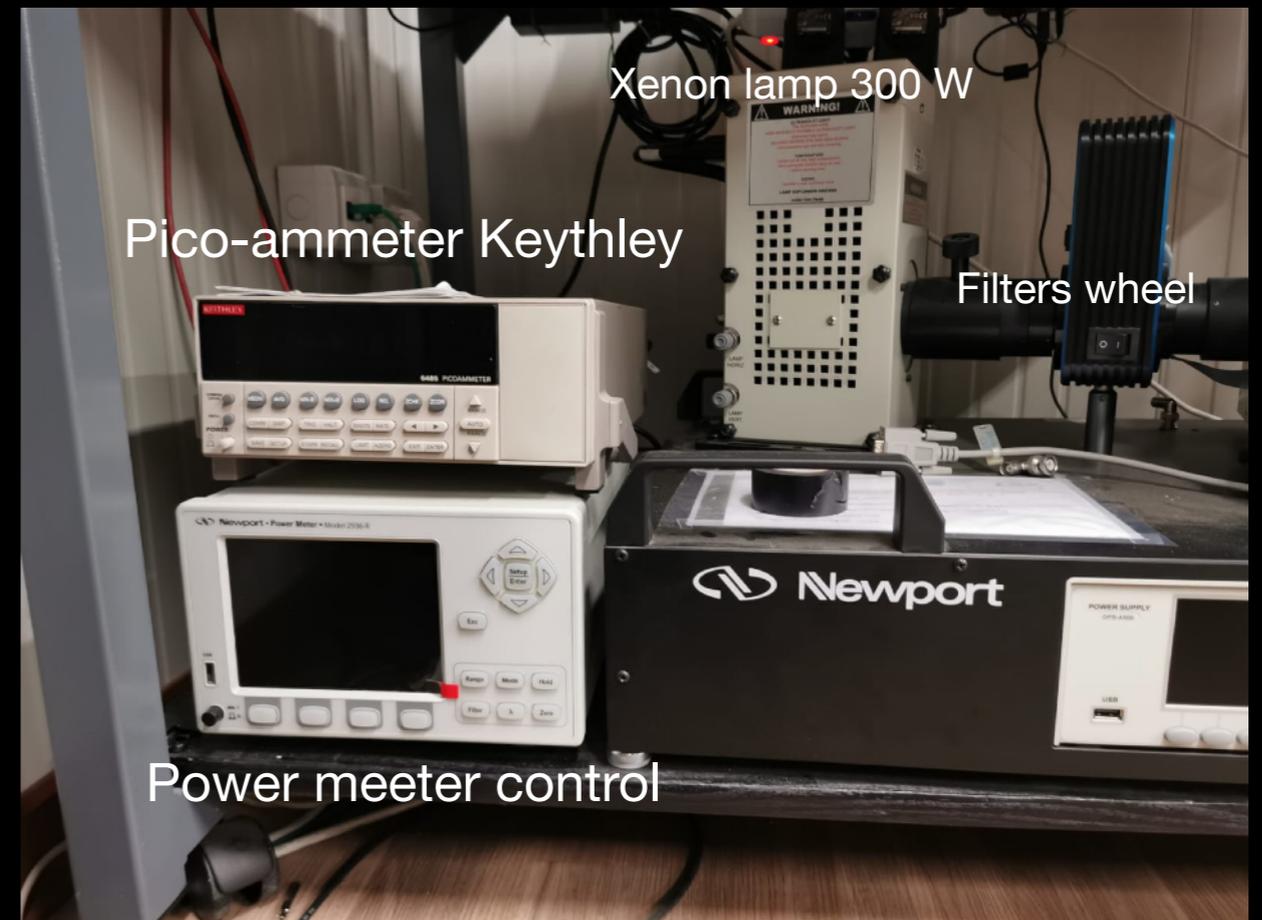




Experimental solutions

- 2D cathode scan is performed by programming the head motion in a comb movement shape.
- Custom code to read the Keithley pico ammeter via RS232 with instrument control toolbox.
- Cathode at -100 V respect to the first dynode grounded together with all the 9 remaining dynodes and anode in order to collect all possible electrons escaping from the first dynode

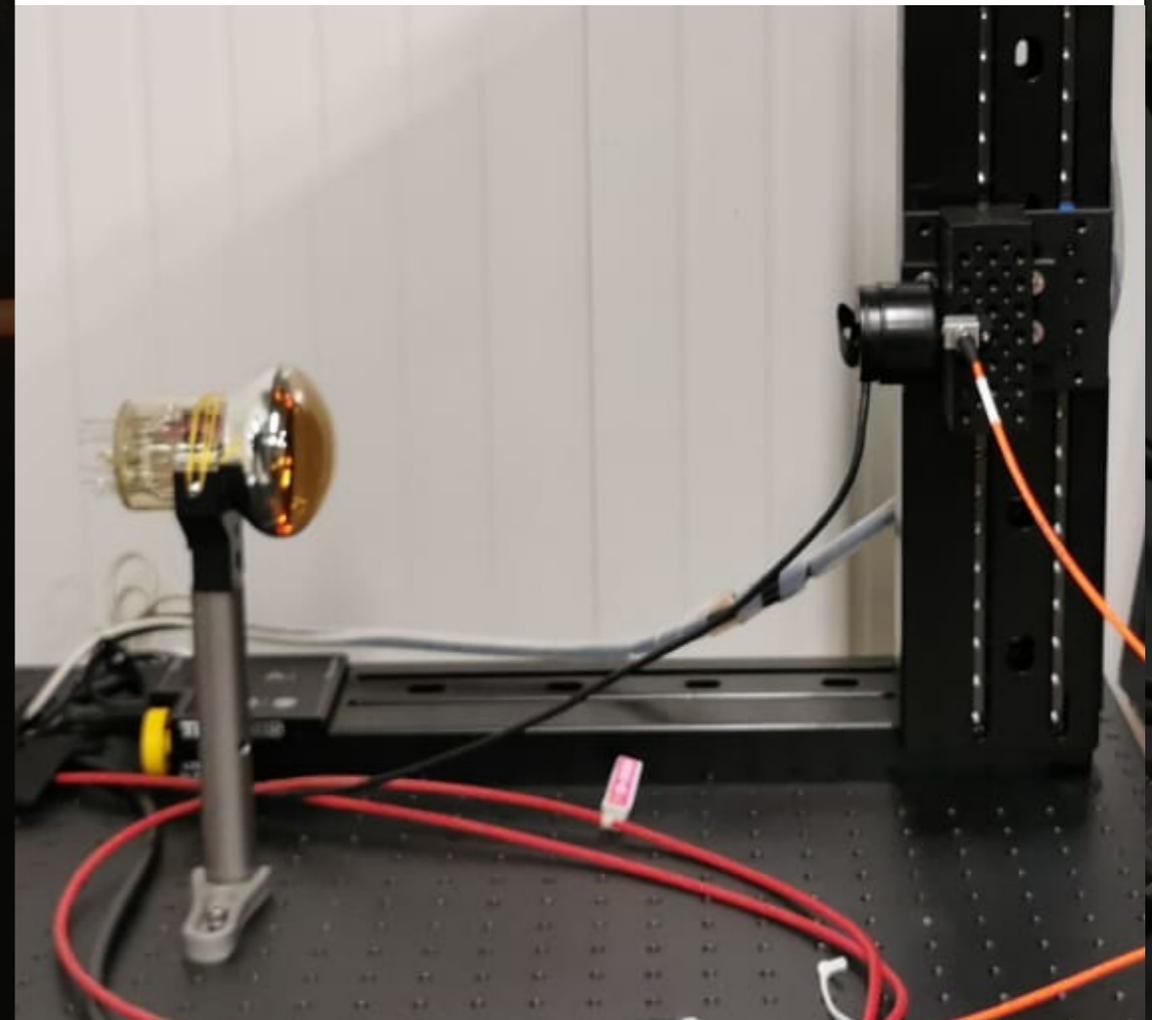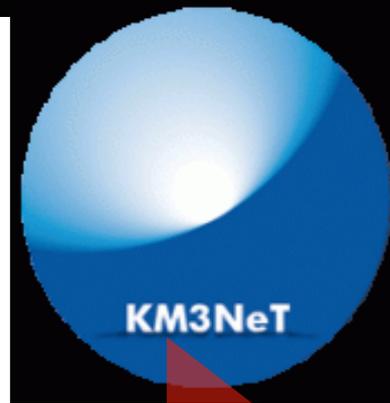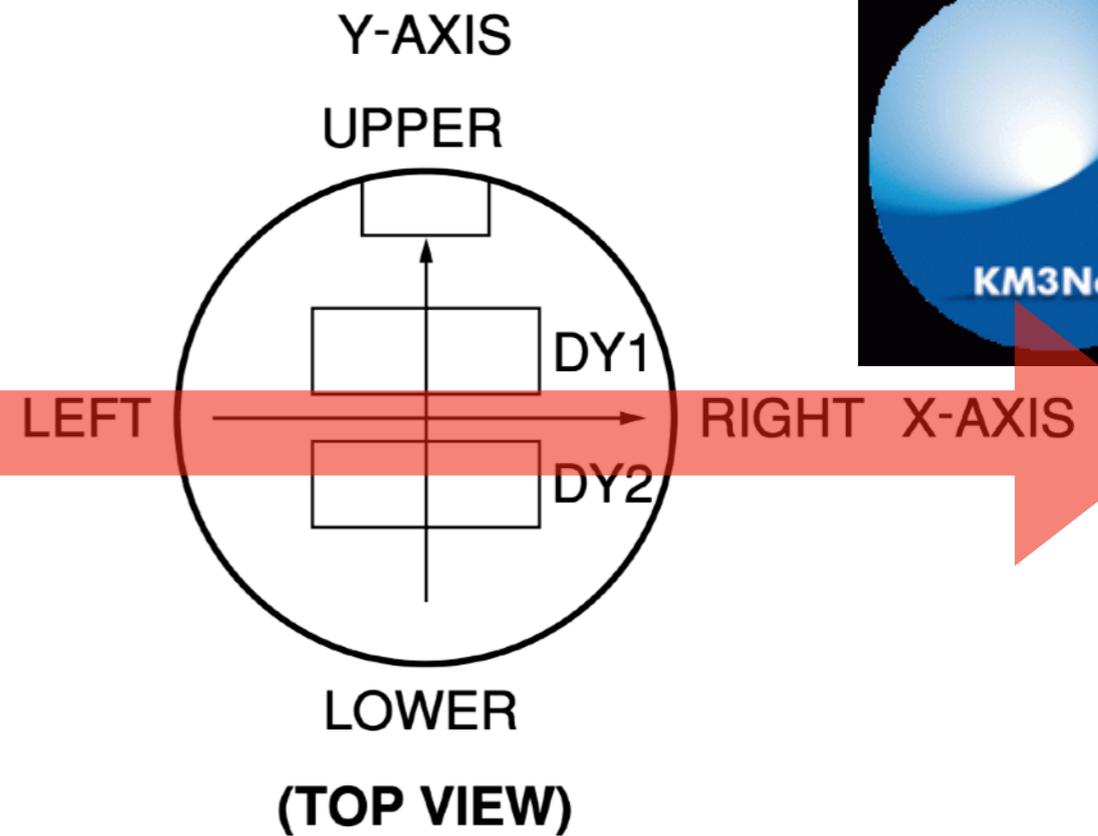


Method

- We acquire a reference power spectrum every ten current spectra and measure PMT current vs Wavelength (use the monochromator scan function) and store it for post processing.

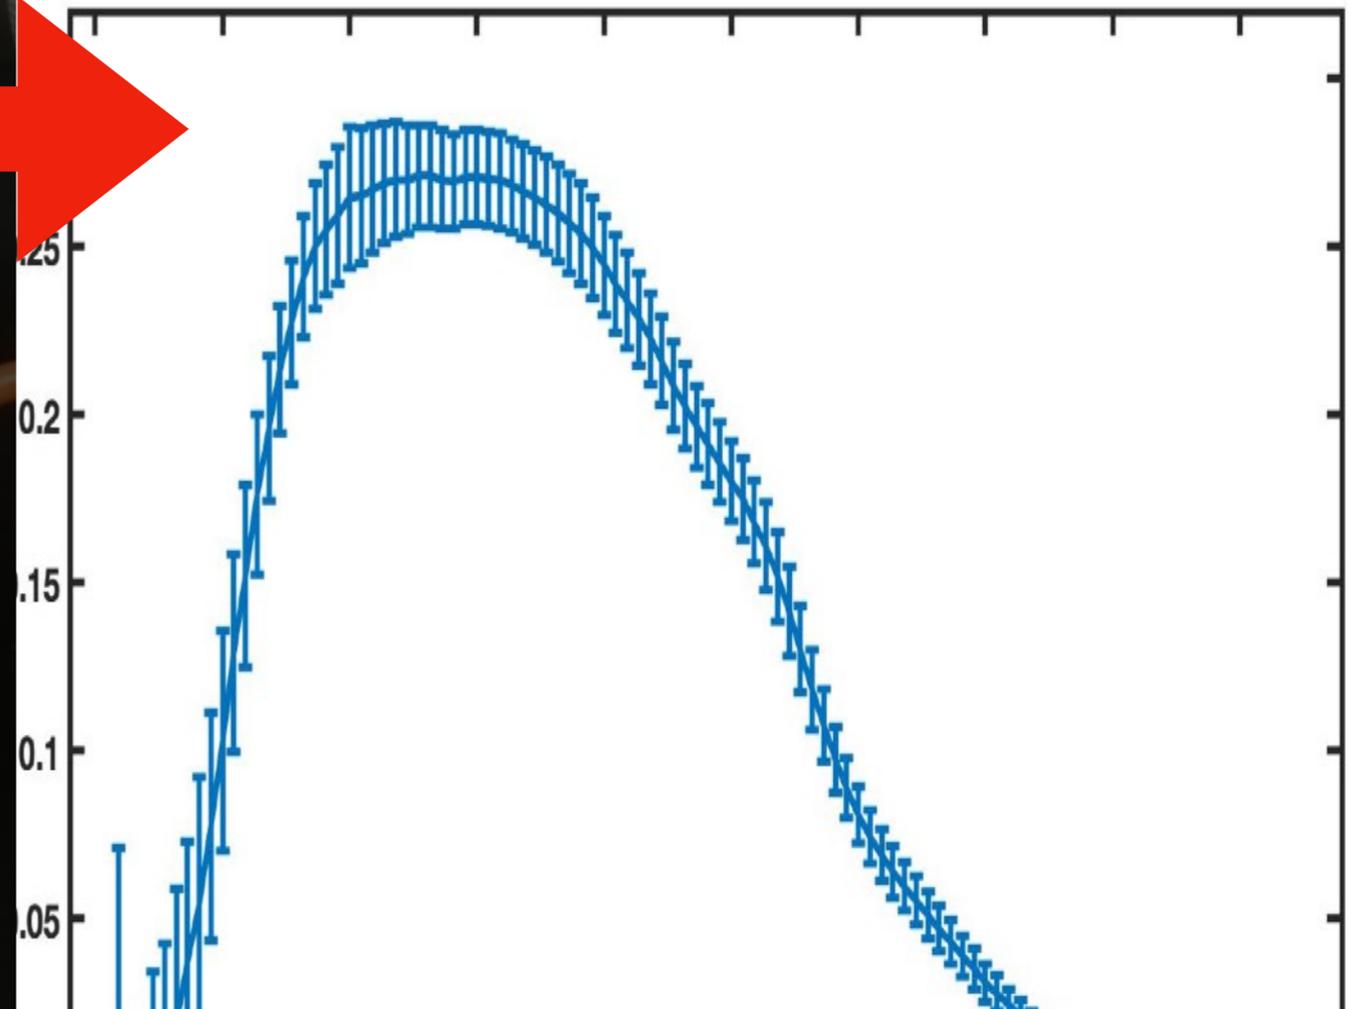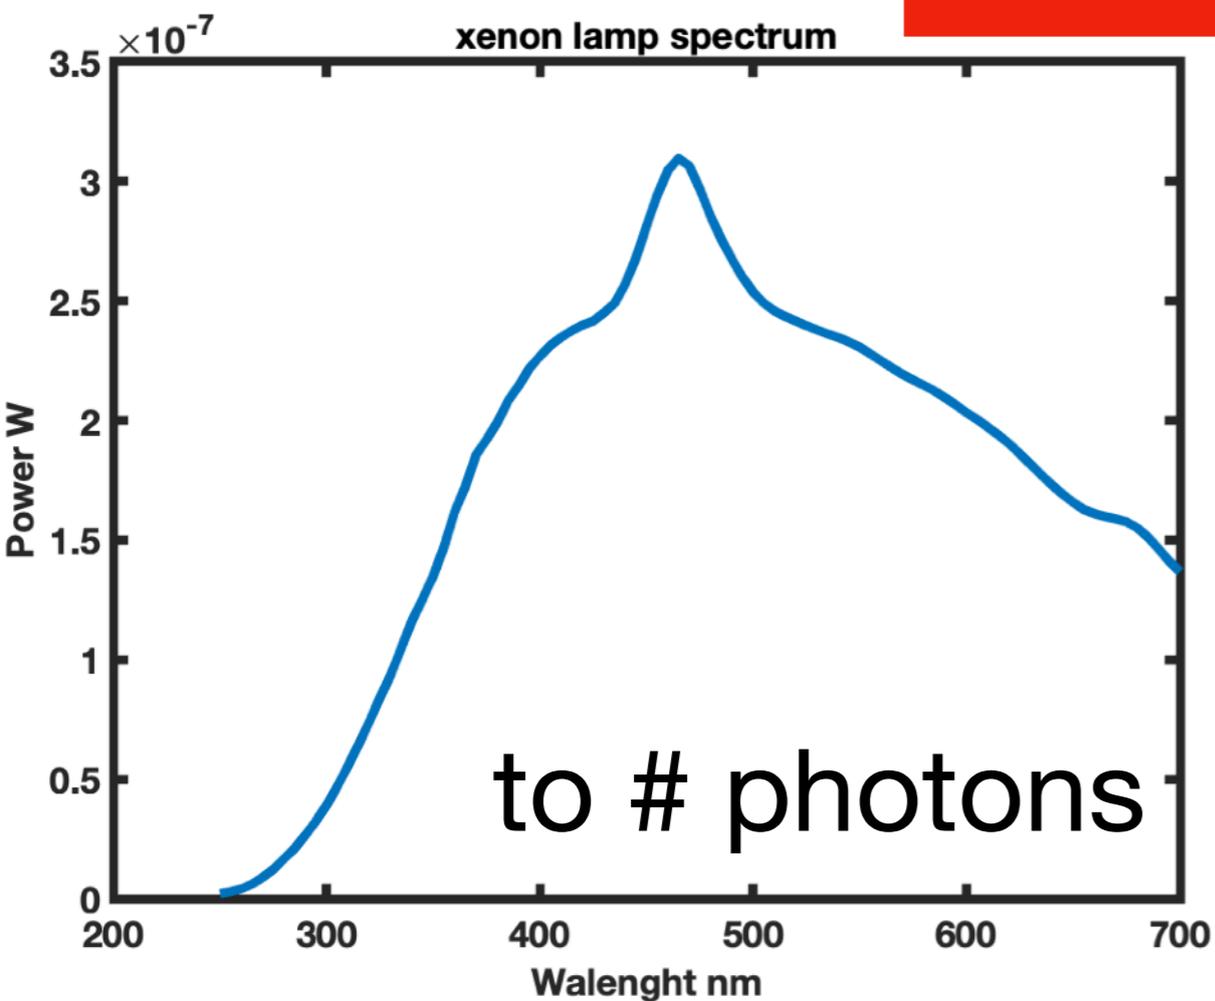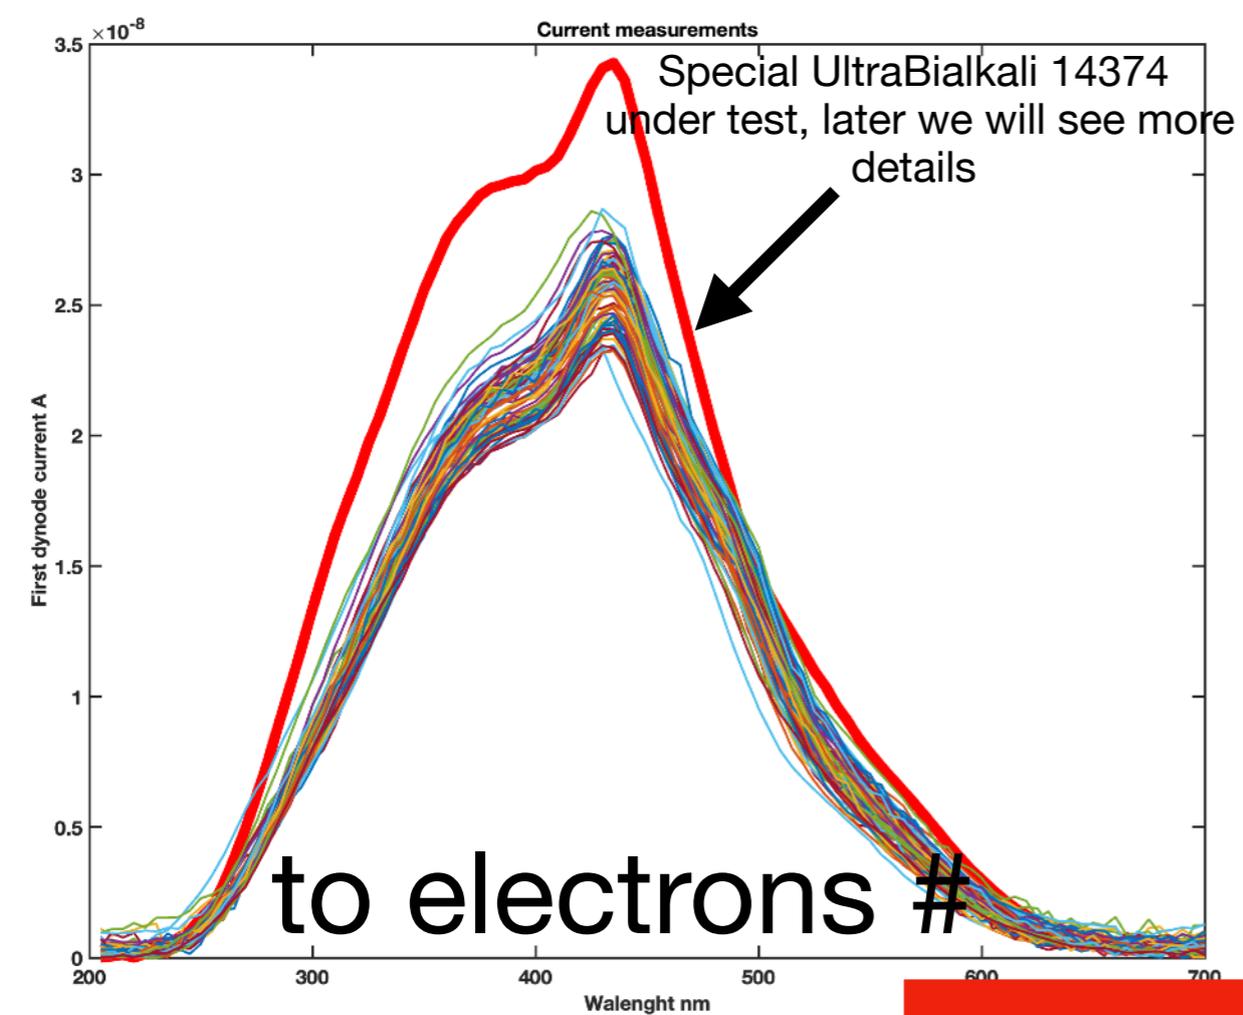

Small subset comparison :
average values of QE for OLD and NEW pmt by using
THE SAME EXPERIMENTAL SETUP

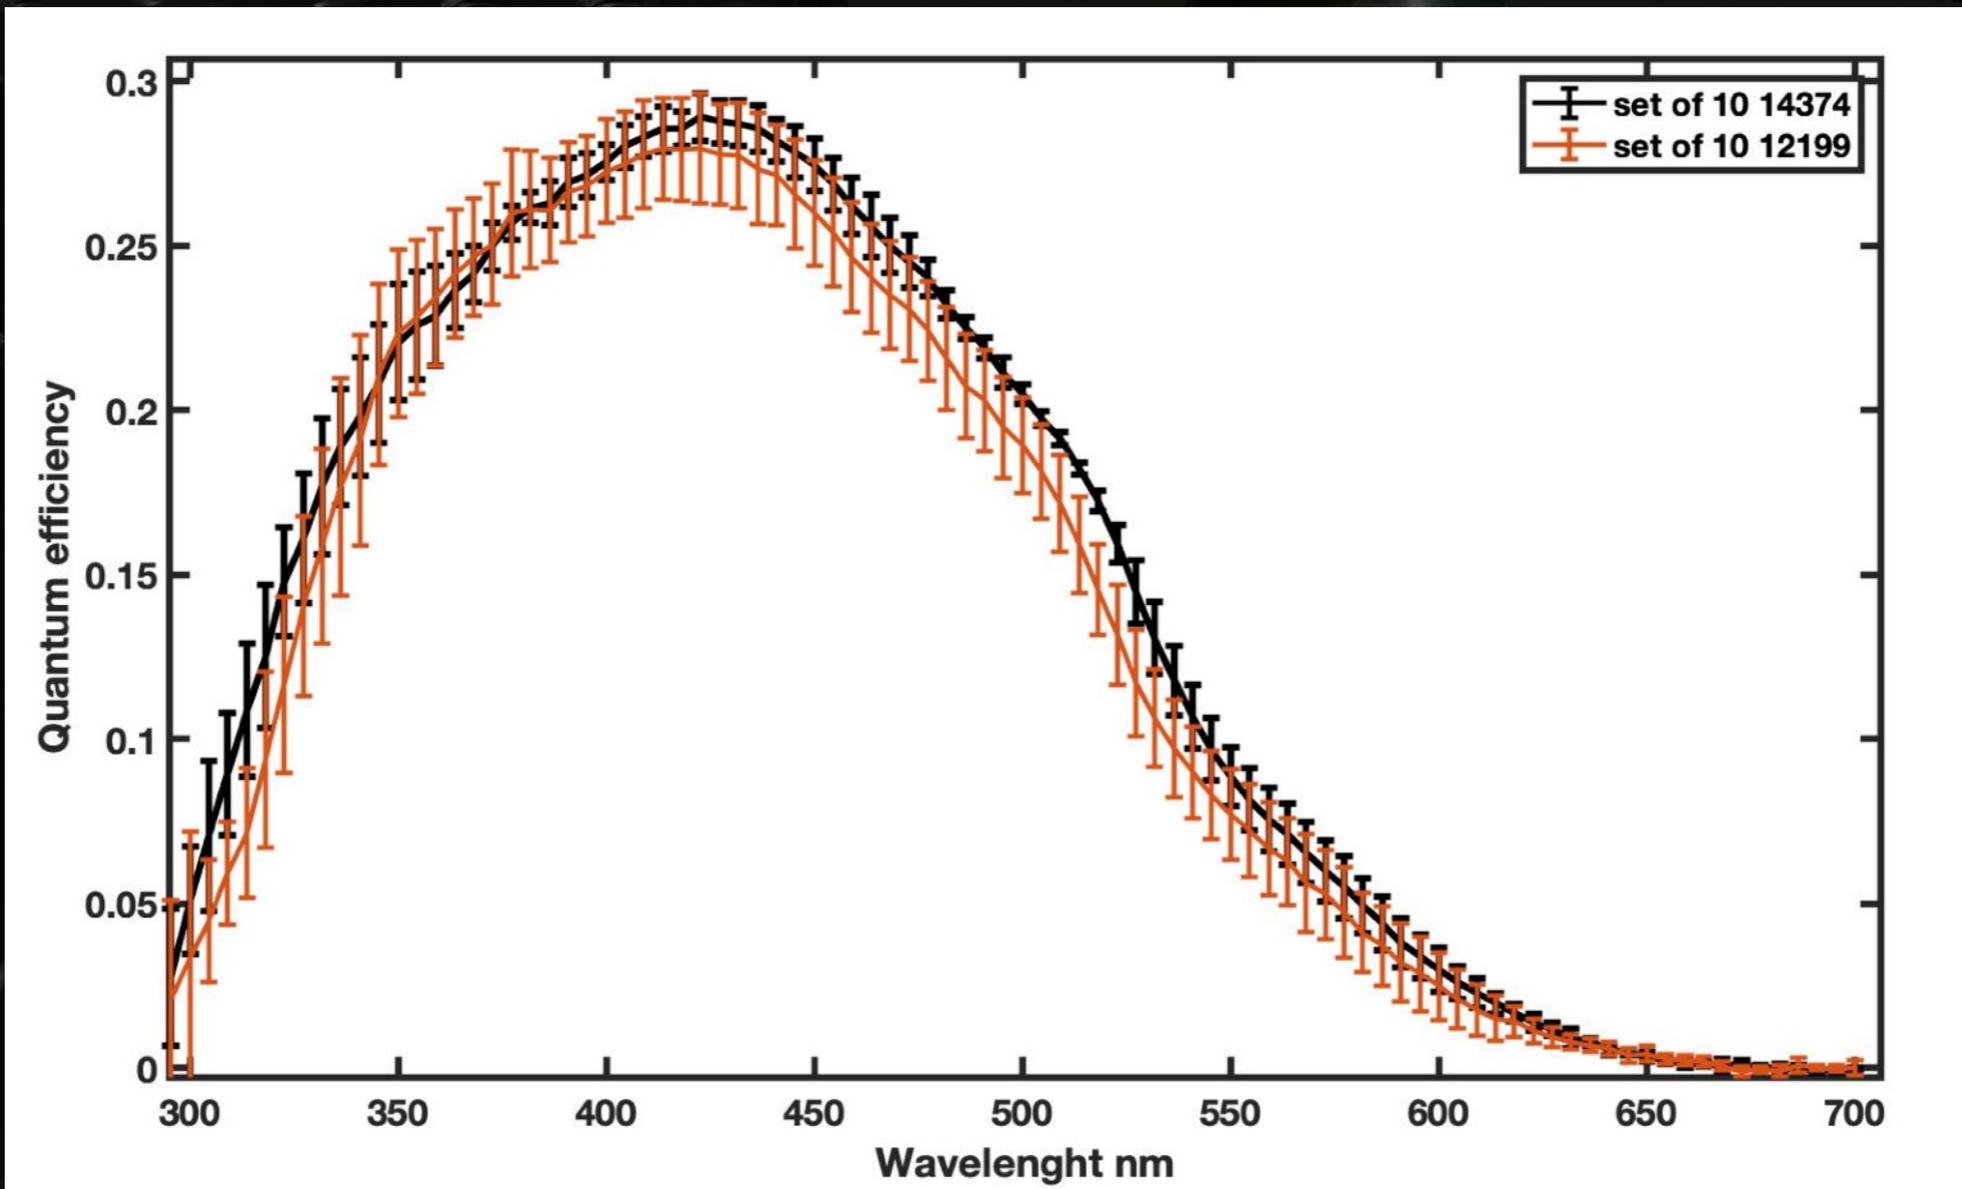

Former measurements on the R12199 performed at ECAP on a 46 pcs. set




Jinst

PUBLISHED BY IOP PUBLISHING FOR SISSA MEDIALAB

RECEIVED: December 29, 2017

ACCEPTED: April 23, 2018

PUBLISHED: May 31, 2018

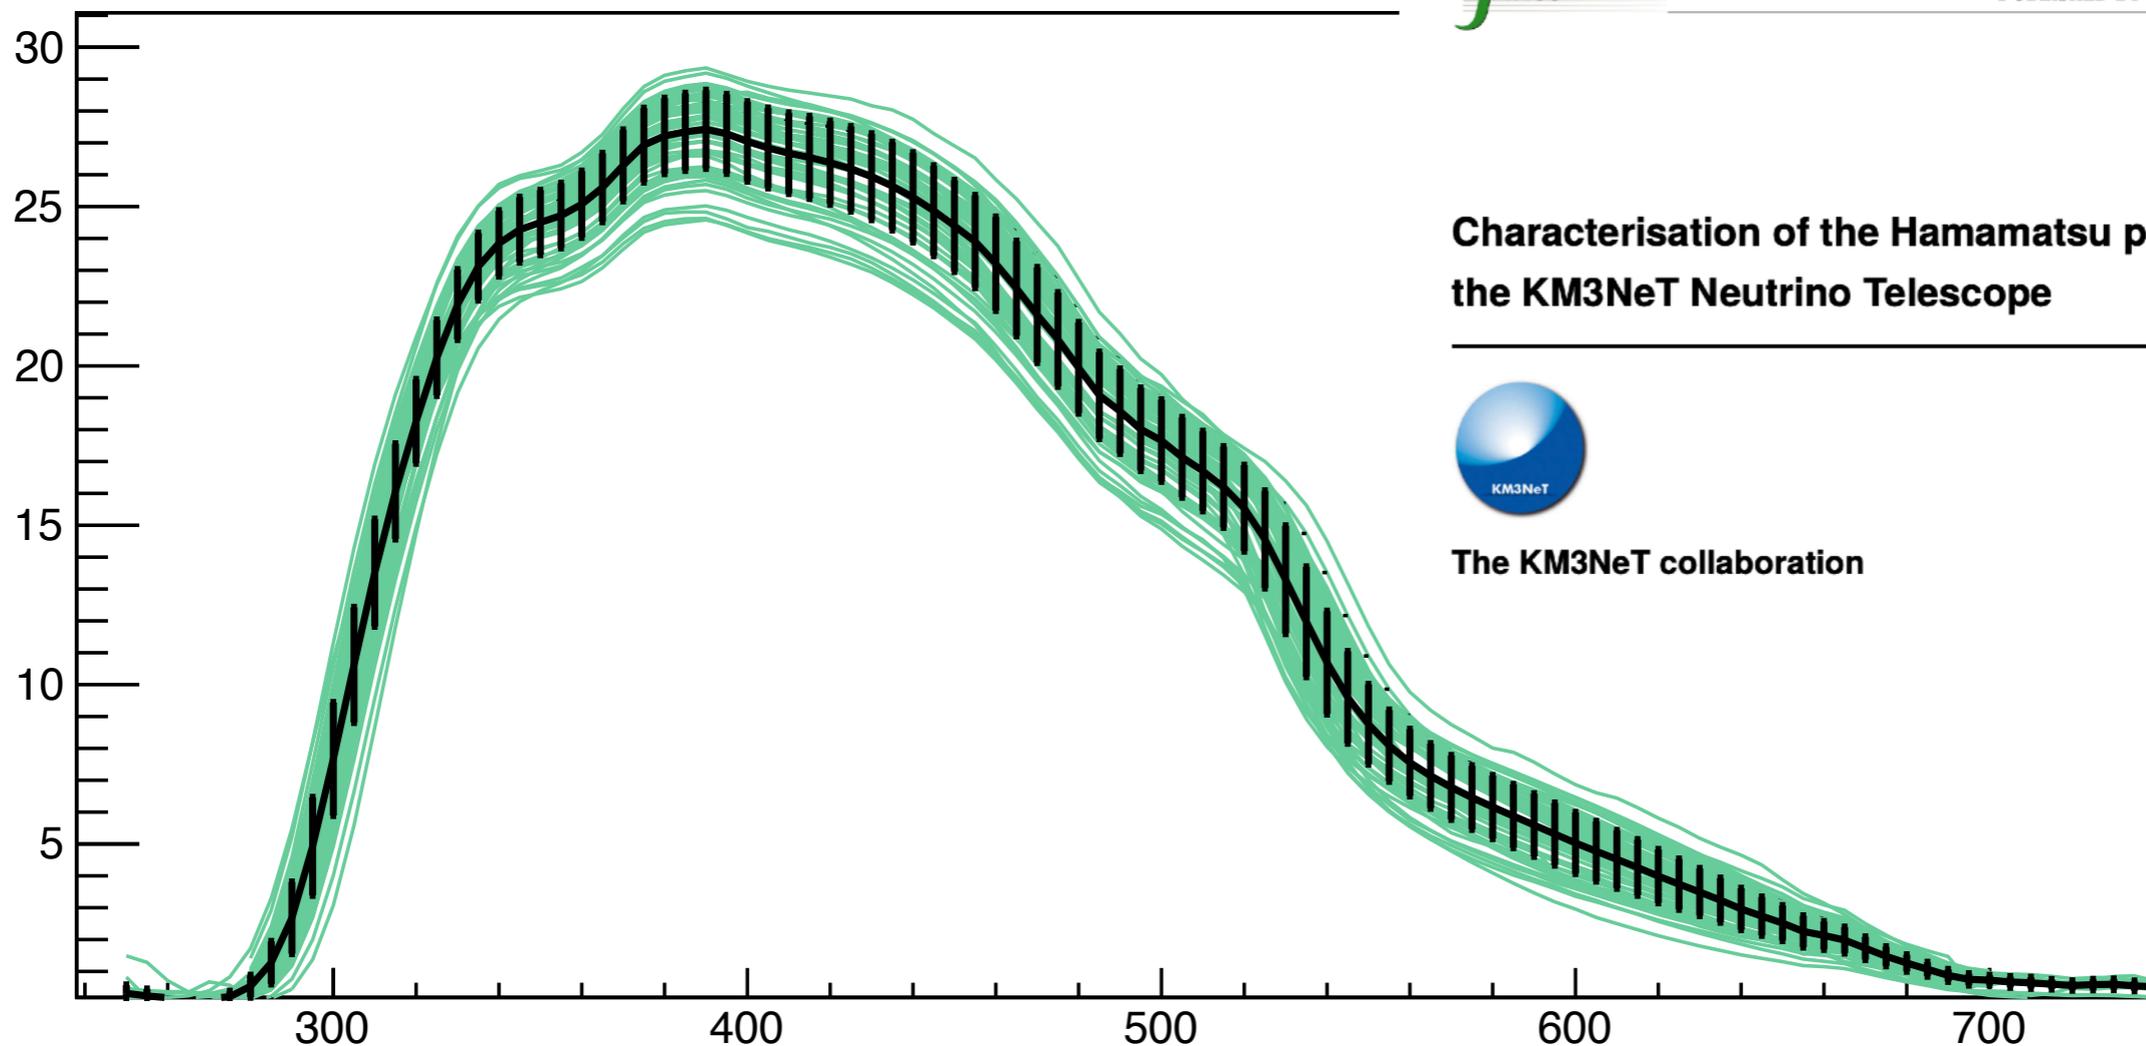



Characterisation of the Hamamatsu photomultipliers for the KM3NeT Neutrino Telescope




The KM3NeT collaboration

Comparing former measurements of ECAP with the new ones performed over a set of 200 PMTs

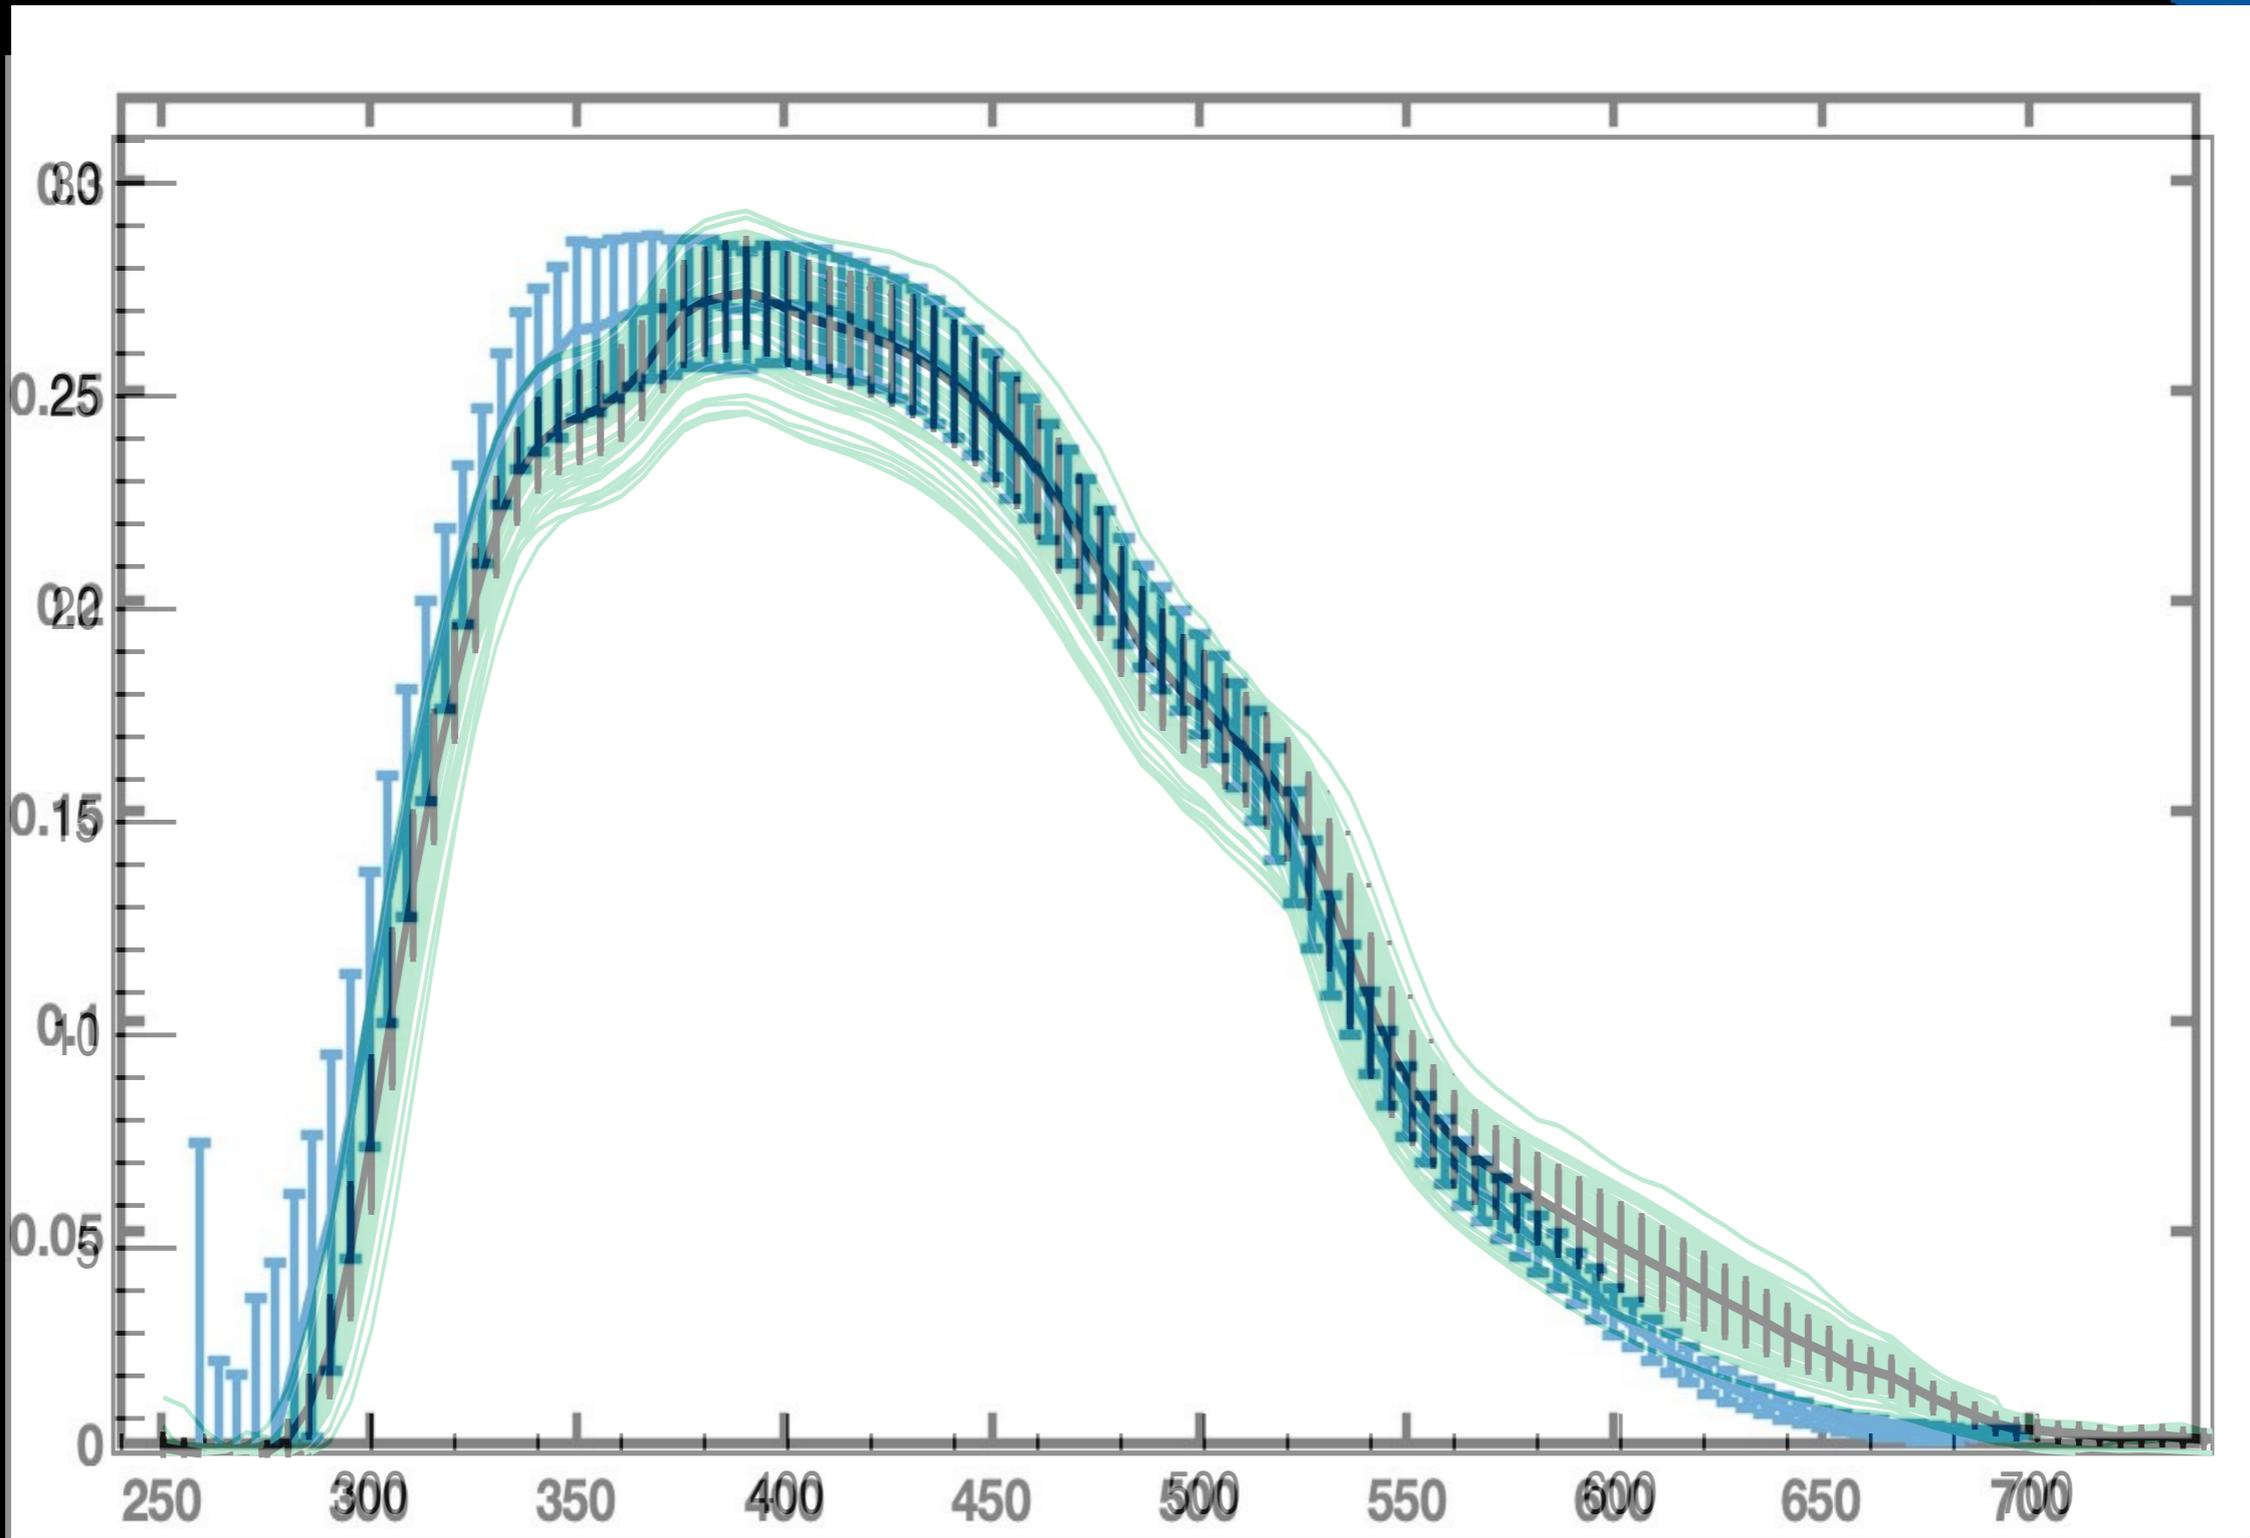

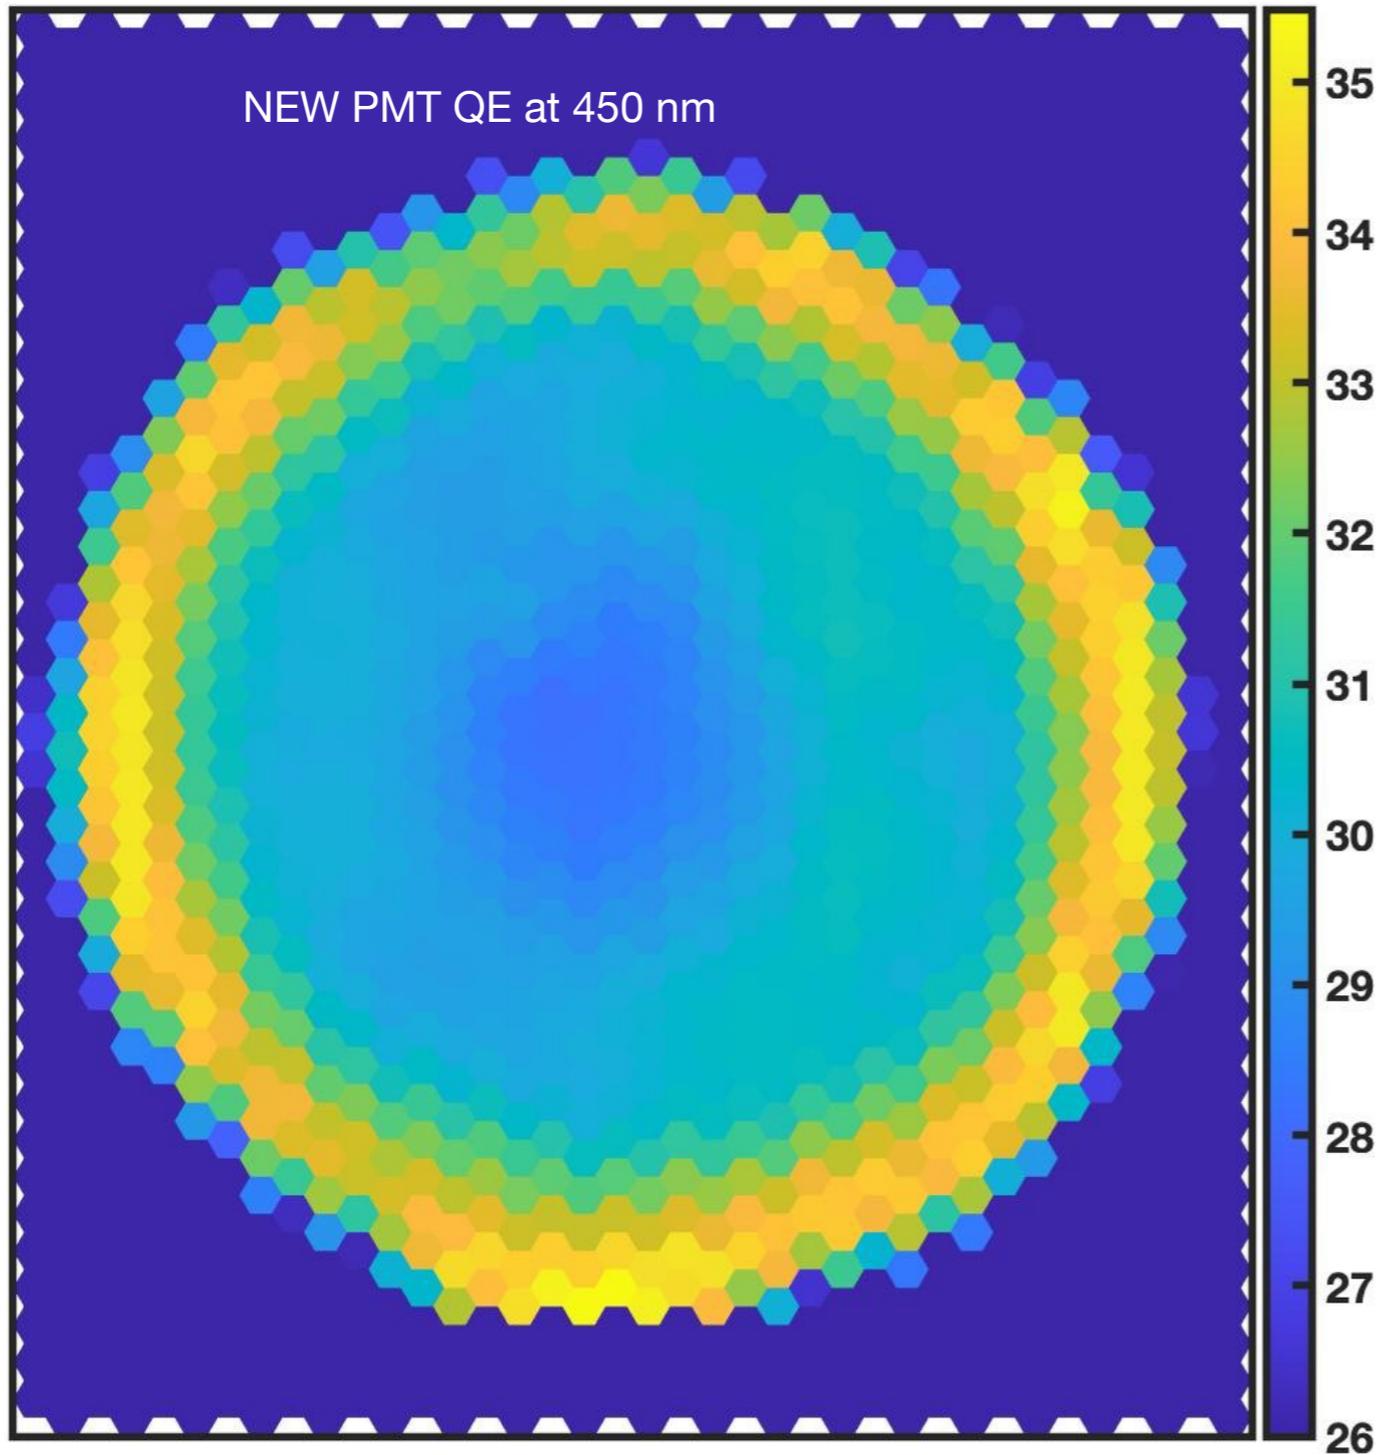


By using the 2D stage it was possible to program and execute the scan of the photocathode. The central part is less sensitive than the borders where there is a clear increase, mainly due to reflected light that stimulates the photoelectric emission twice.

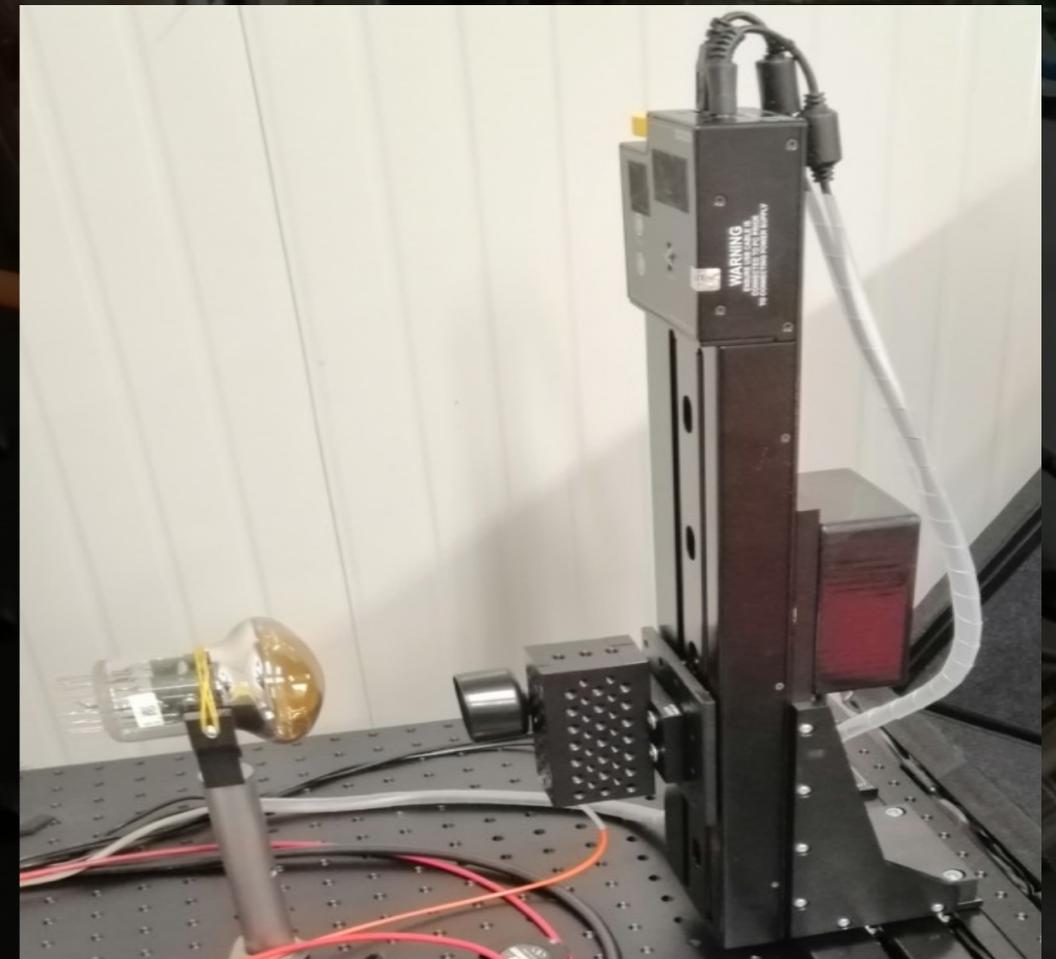


Evidences:

- The QE is minimal at the center at normal incidence
- The inner borders of the PMT “mushroom” is internally coated with a metal sheet (i.e a perfect mirror for all the wavelengths)
- This effect is documented by producers but not fully explained

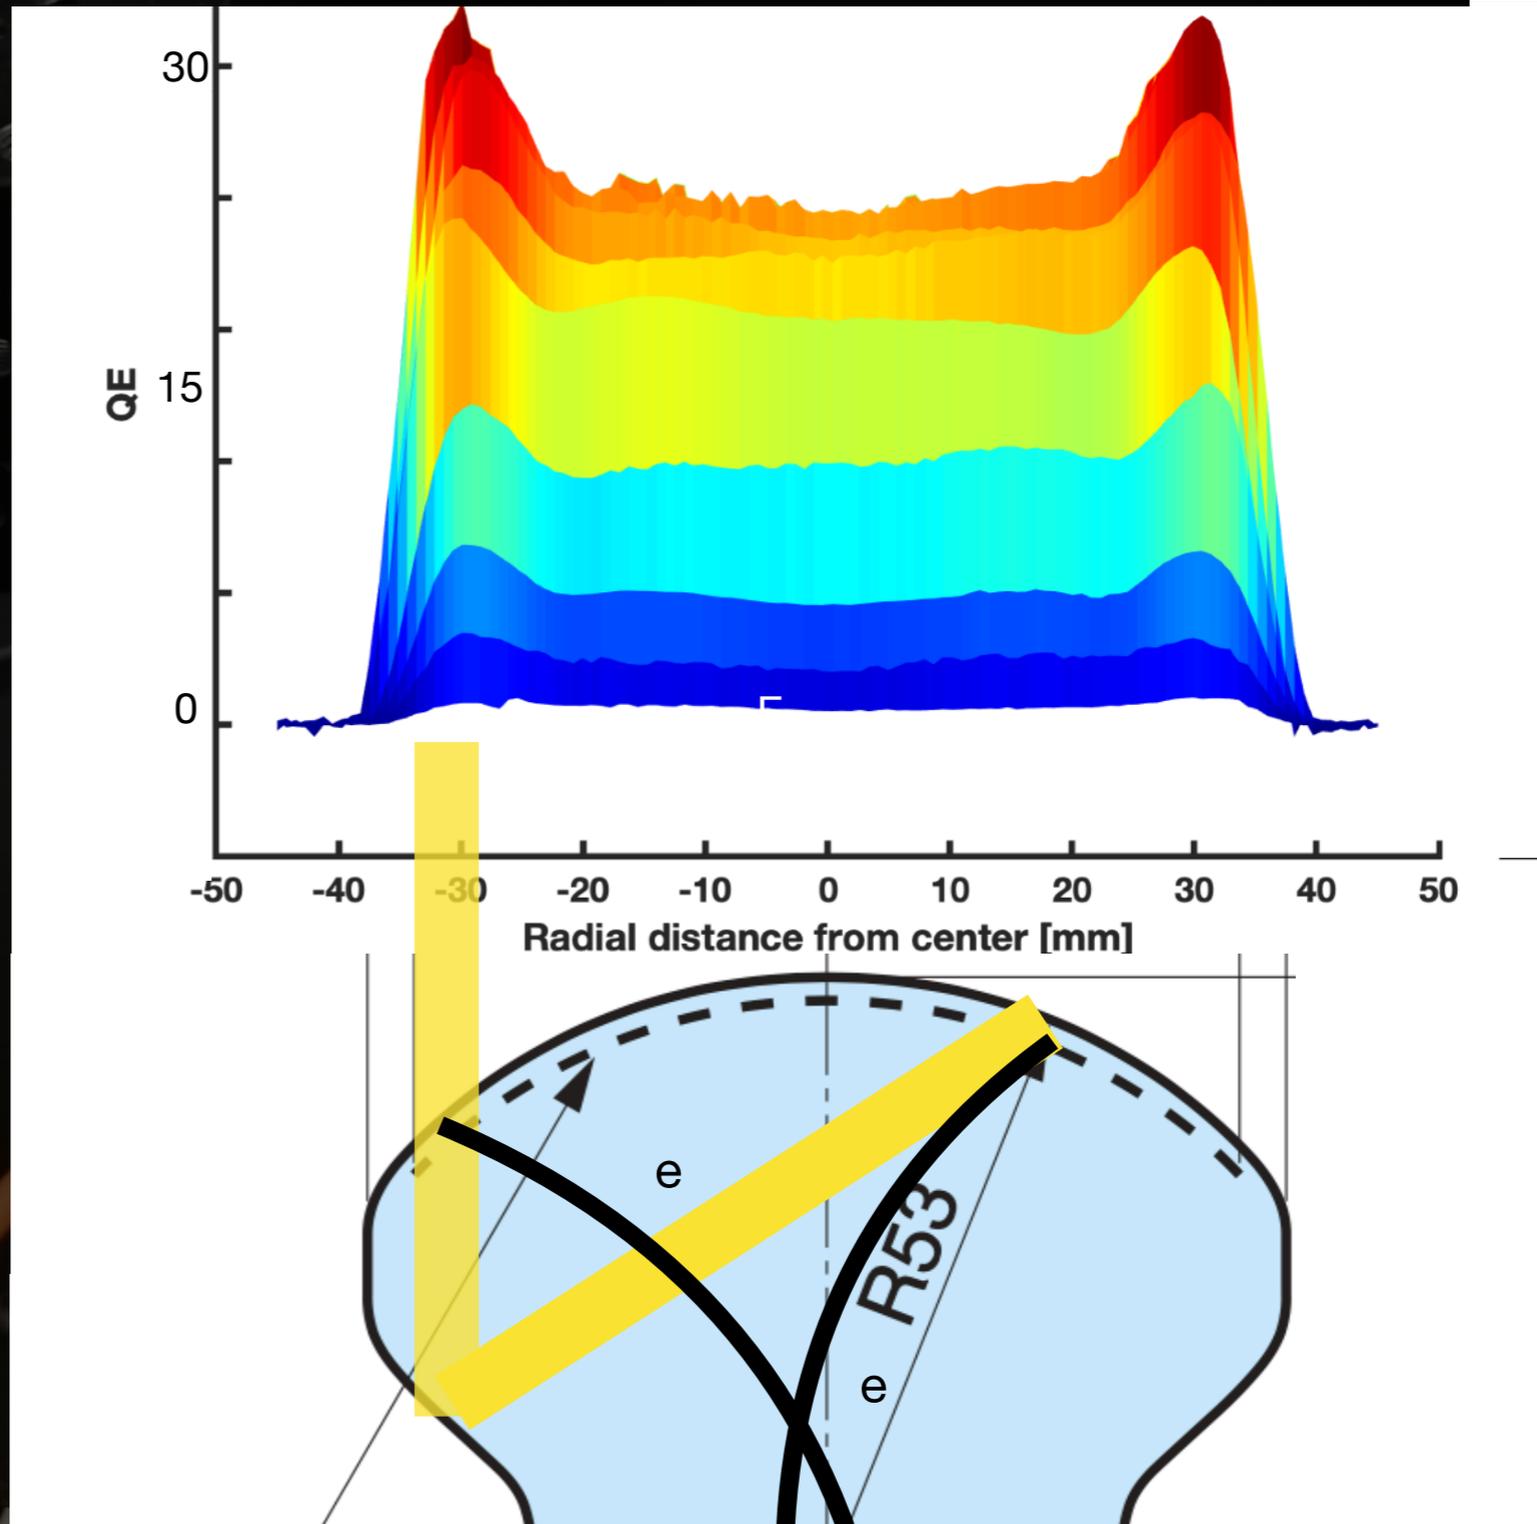

Radial homogeneity comparison between old (red) and new (blue) PMTs

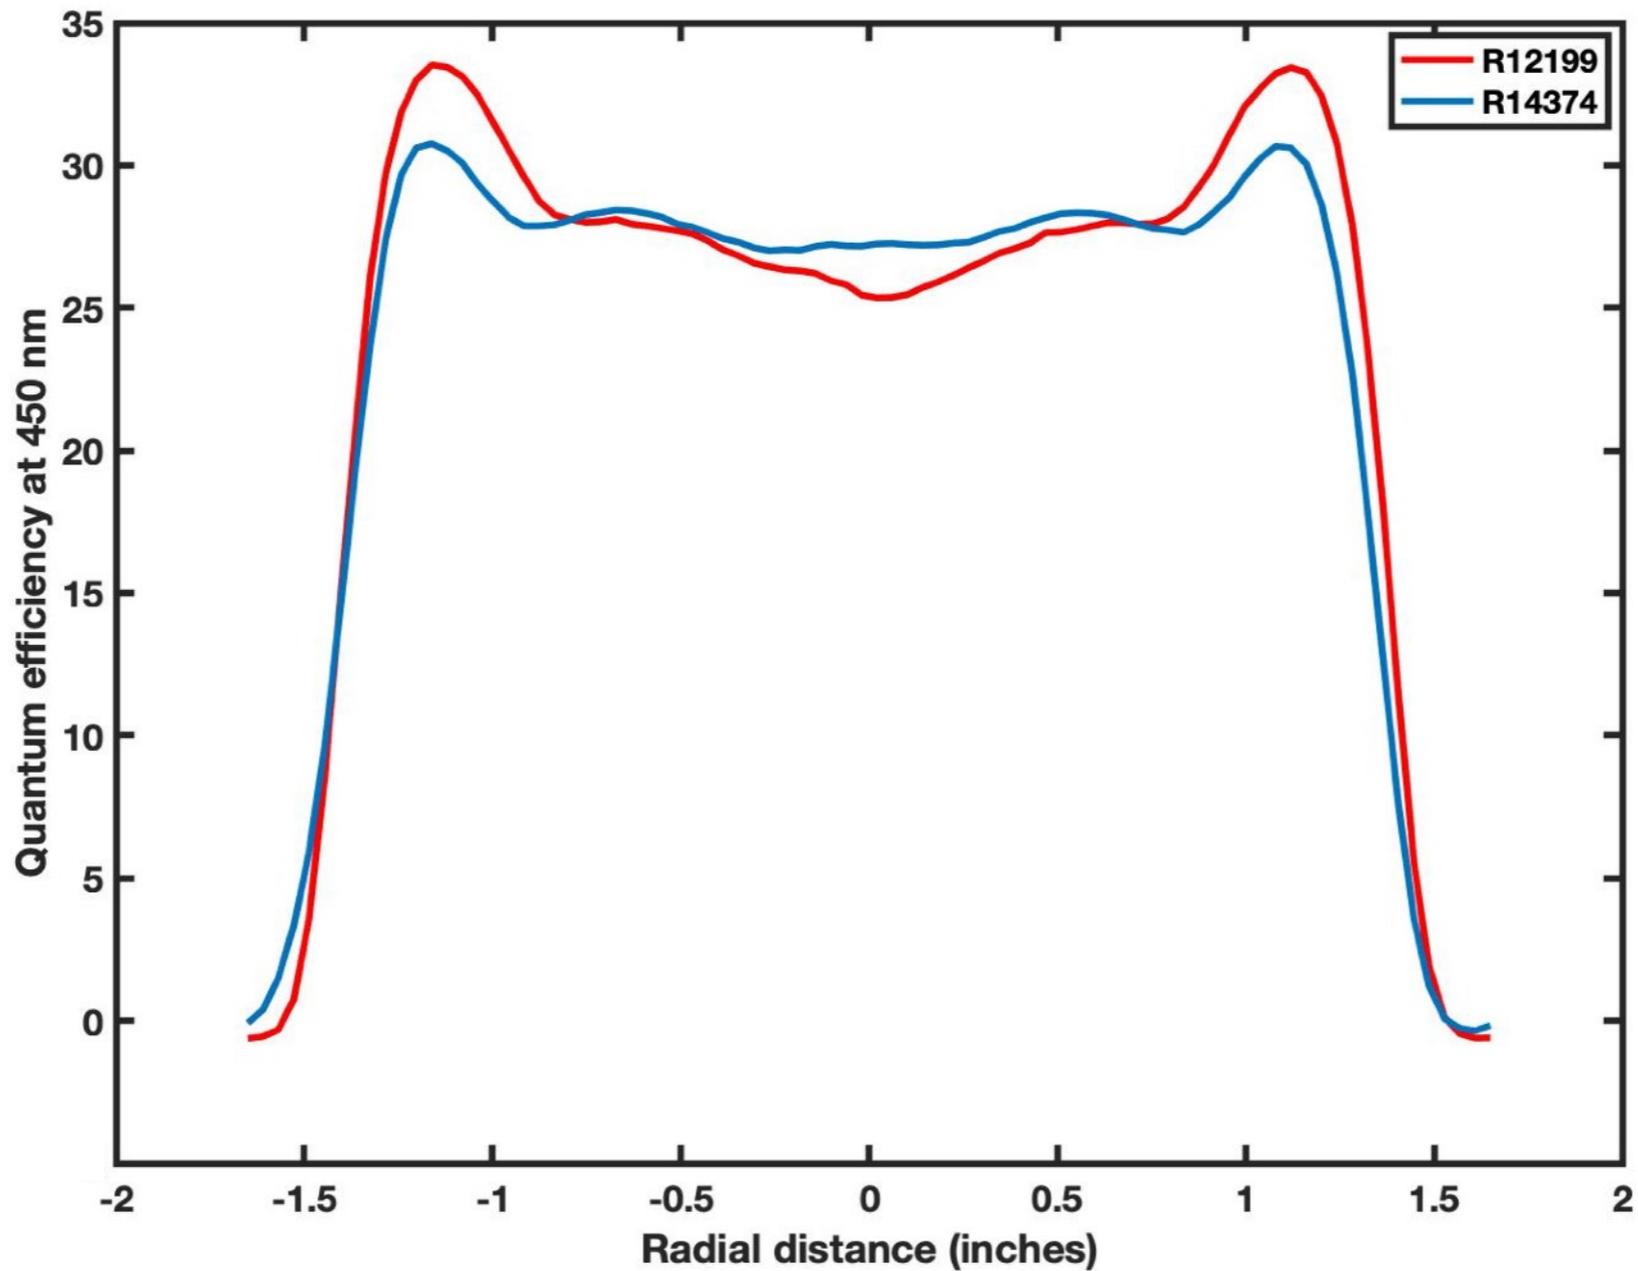

Nuclear Instruments and Methods in Physics Research A 623 (2010) 276–278

Contents lists available at ScienceDirect

Nuclear Instruments and Methods in
Physics Research A

journal homepage: www.elsevier.com/locate/nima



Latest bialkali photocathode with ultra high sensitivity

Kimitsugu Nakamura*, Yasumasa Hamana, Yoshihiro Ishigami, Toshikazu Matsui

Hamamatsu Photonics K.K. Electron Tube Division, Shimokanzou 314-5, Iwata, Shizuoka 438-0193, Japan

ARTICLE INFO

ABSTRACT

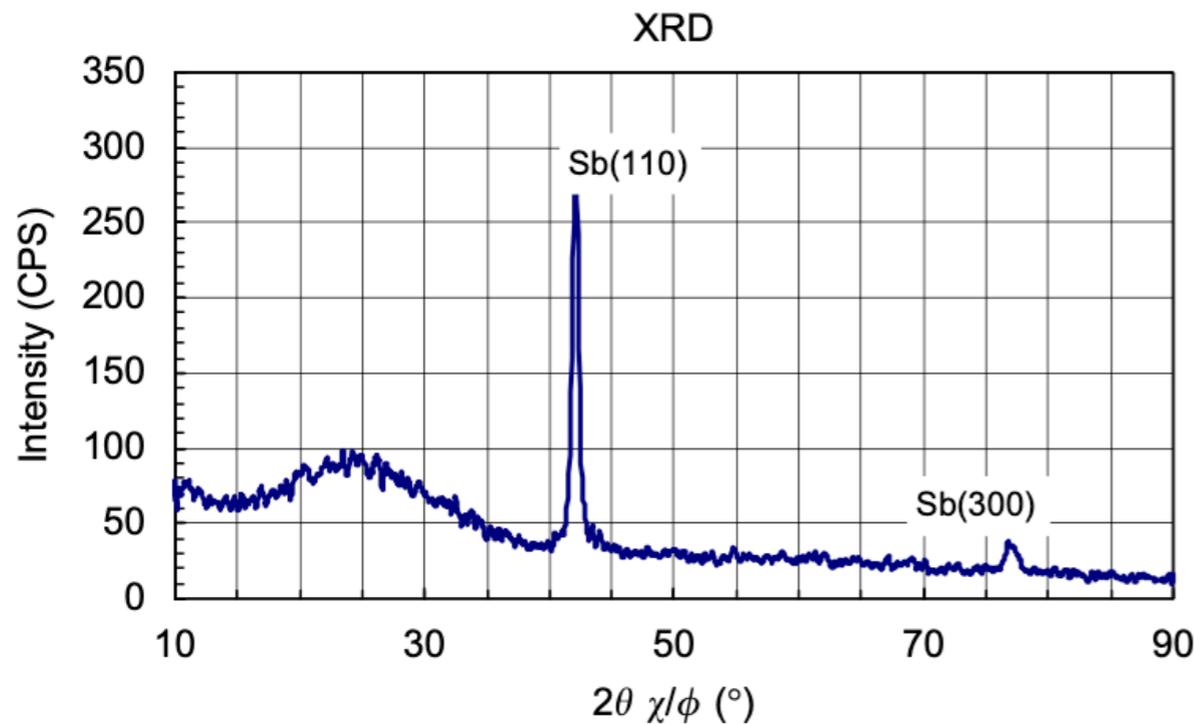


Fig. 1. The X-ray diffraction analysis result of Sb thin film.


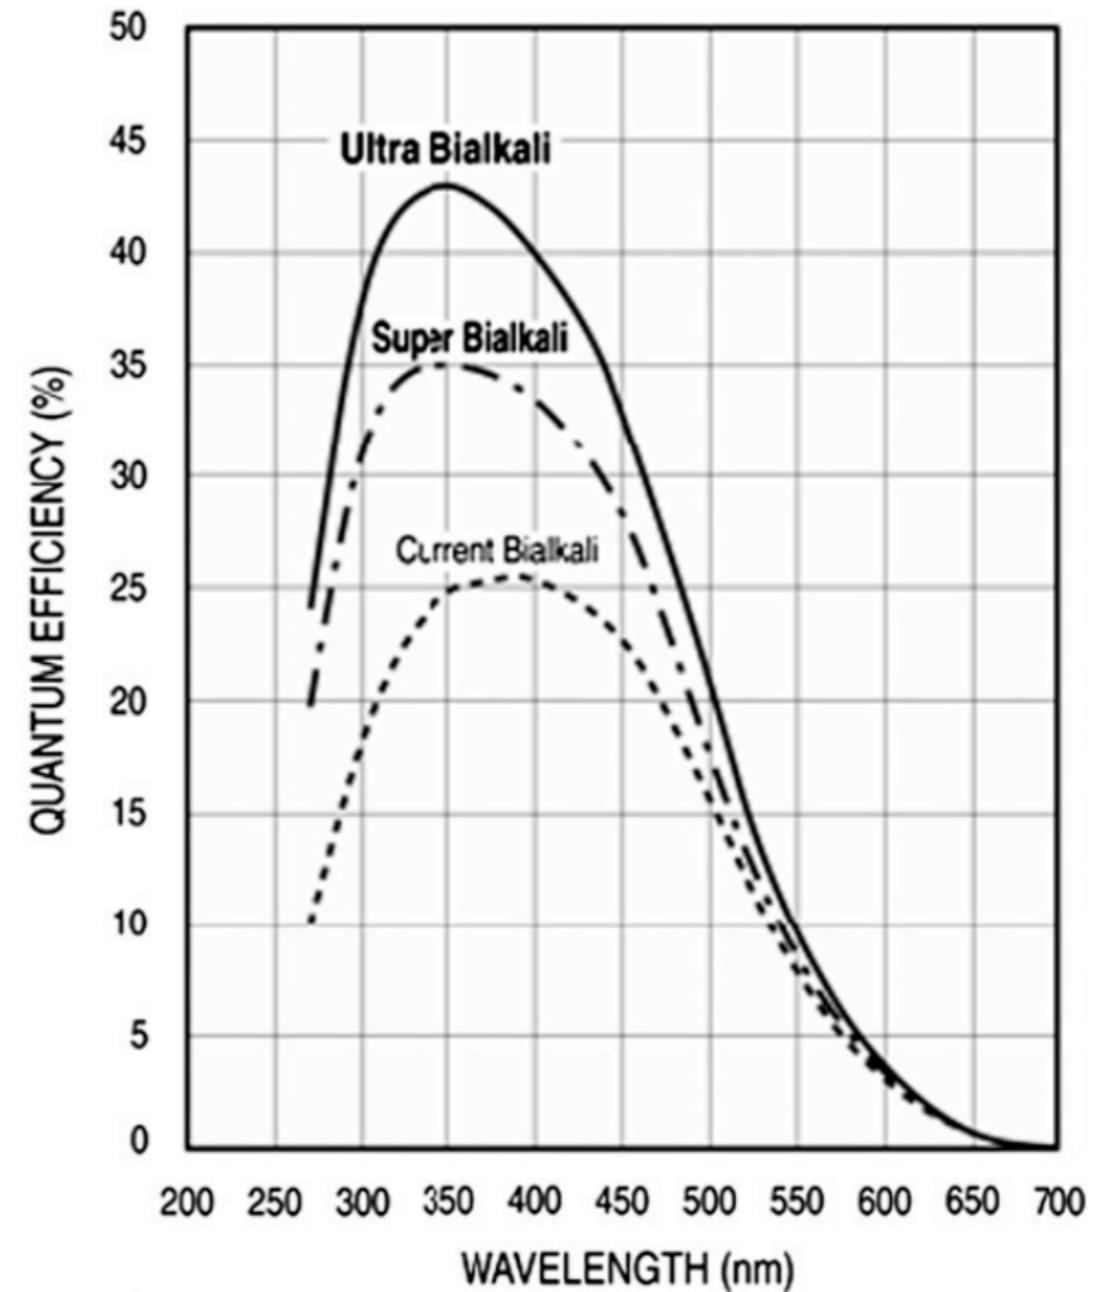


Fig. 2. Typical QE curves for UBA, SBA and standard bialkali photocathodes.

Crystallinity of the Antimony coating plays the fundamental role of improving QE in bialkali photocathodes

A special version with increased QE
is under test

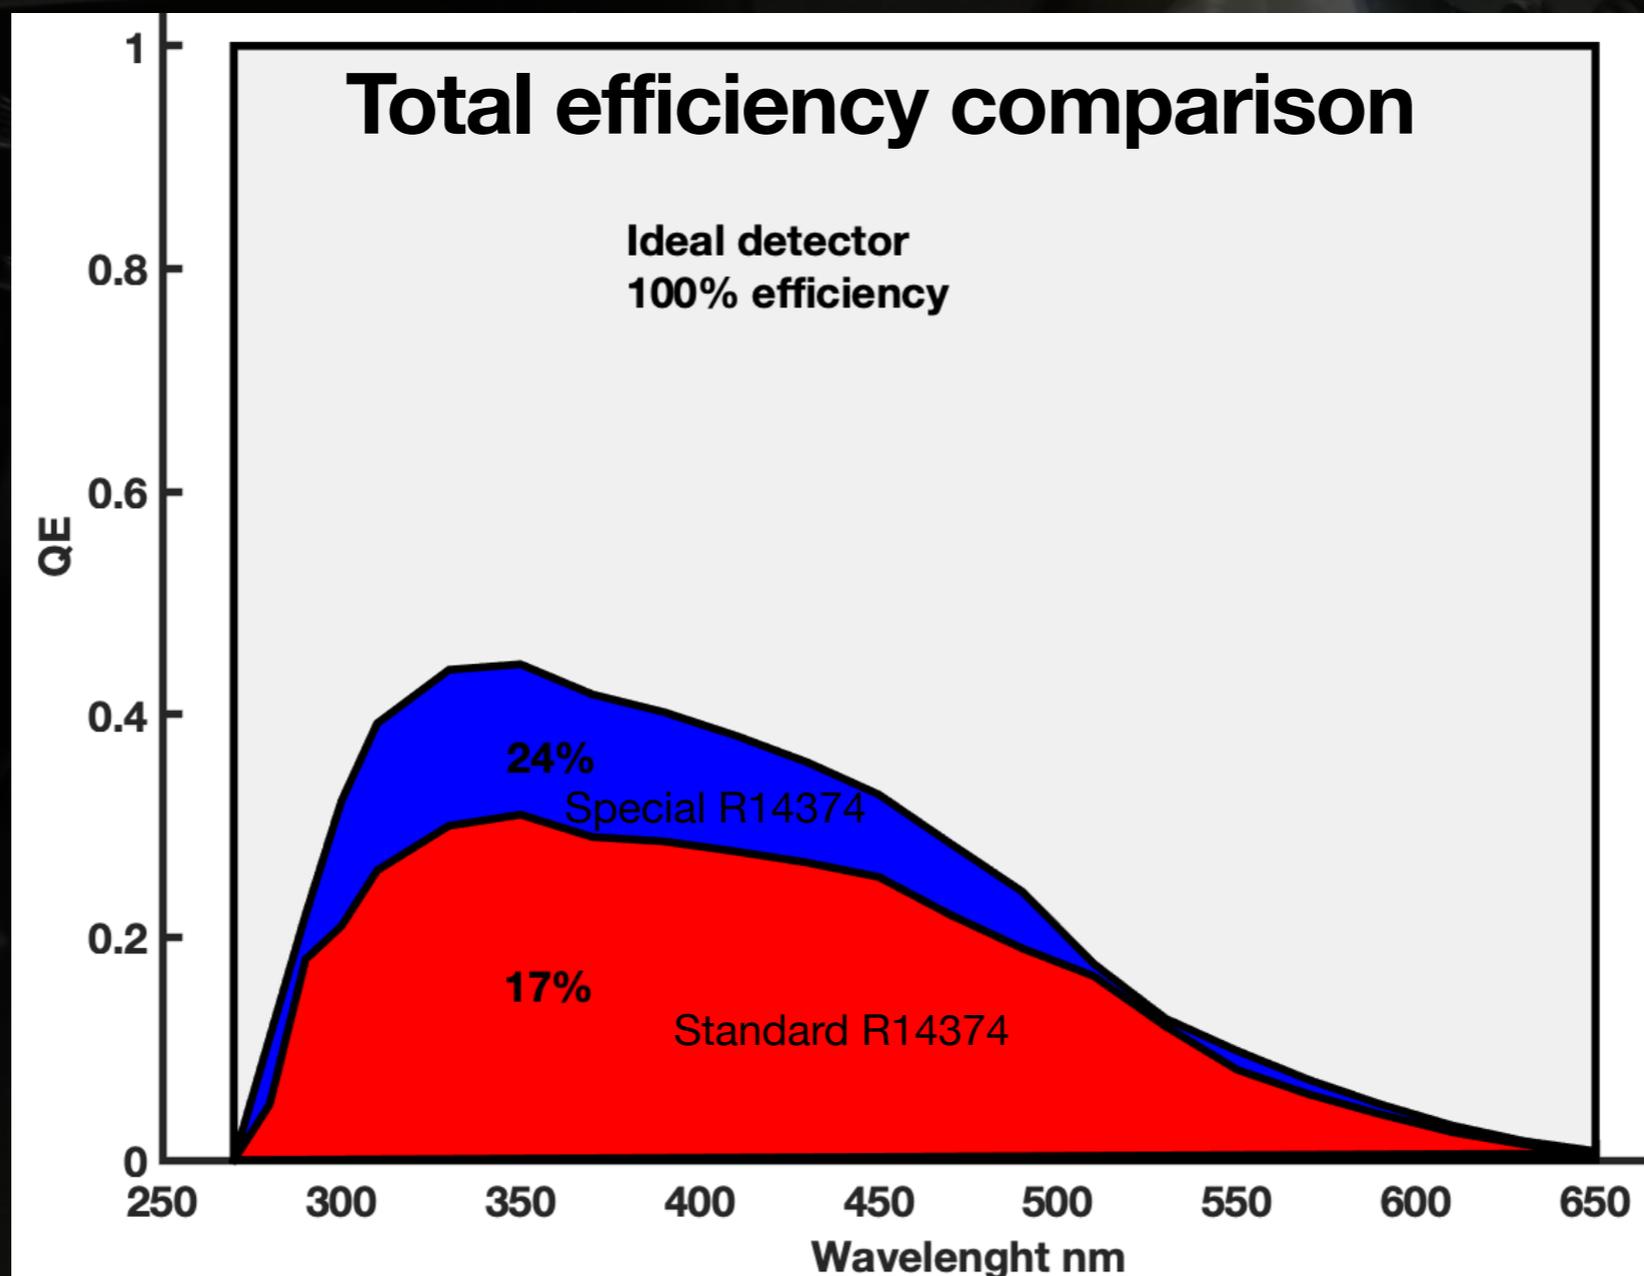

+41%



M.C. Mollo et al.

**The Dark Box instrument for fast automatic testing of the photomultipliers for KM3NeT
Volume 236 - The 34th International Cosmic Ray Conference (ICRC2015)**

- **After-pulses**: *are spurious pulses that appear in the wake of true pulses. they can limit the number of true pulses that can be registered.*

After-pulses have two main causes:





- (a) light emitted by electrodes due to electron bombardment.*
- (b) ionisation of residual gas traces.*

- **Dark counts**: *A small amount of current flows in a photomultiplier tube even when operated in a completely dark state.*


- (c) Thermionic emission*
- (d) Leakage current*
- (e) Photocurrent produced by scintillation from glass envelope or electrode supports*
- (f) Ionisation current from residual gases (ion feedback)*

- **The transit-time spread**: *variations in the single photoelectron transit time*

DarkBox test summary (Test #14374_12)
 PROMIS ID: 007C3D
 Quality : GREEN
 UPI : UNKNOWN
 Tuned HV : -1007.16 V
 DarkRate : 432.07 Hz
 ToT peak : 27.4373 ns
 Prepulses : 0.000218372%
 Delayed : 1.75792%
 Afterpulses : 3.05738%
 TT peak (fit): 18.7193 ns
 TT FWHM (fit): 2.37092 ns
 TT peak : 19 ns
 TT FWHM : 2 ns

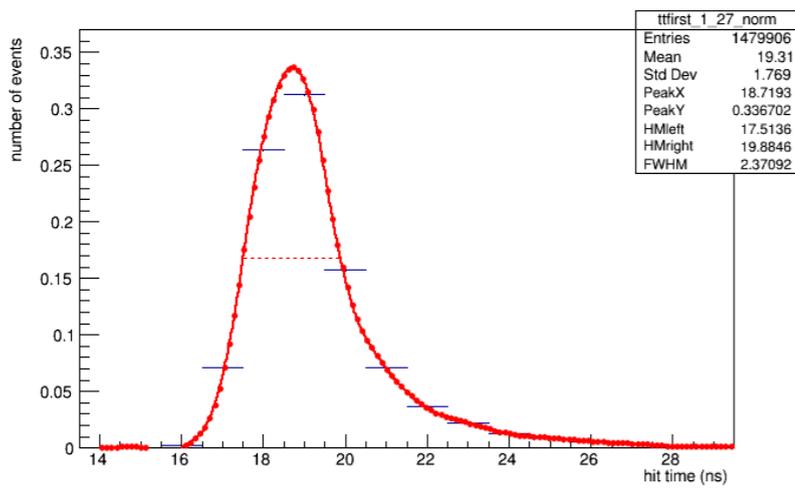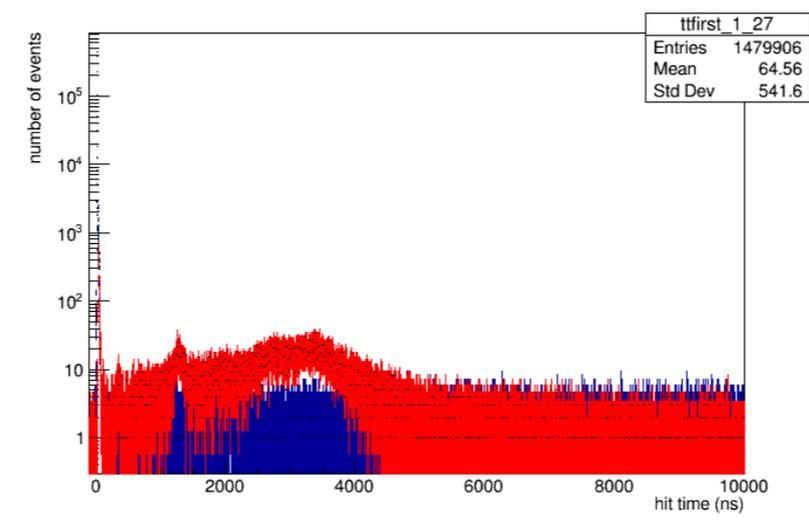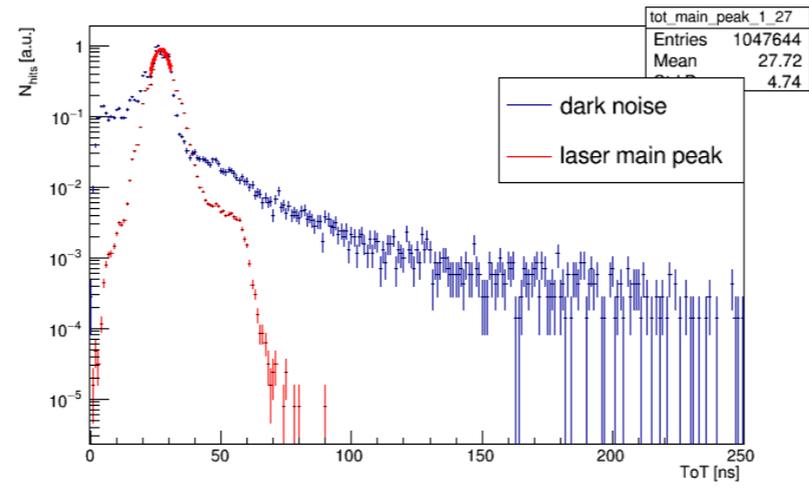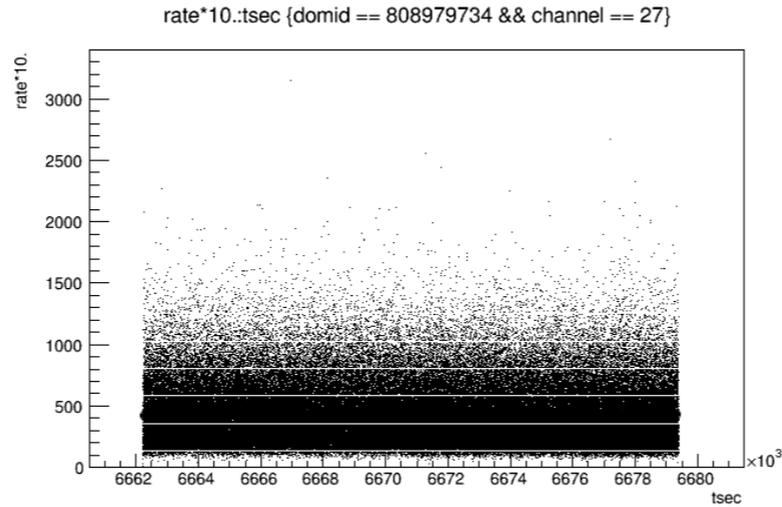

HV tuning

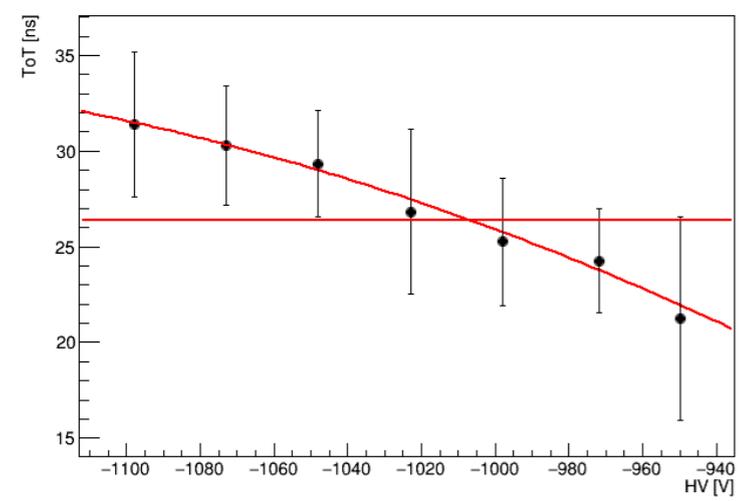


Time properties and dark counts are studied by means of the Dark Box instrument using the digital base





After-pulses measurements



between 100 ns and 10 μ s

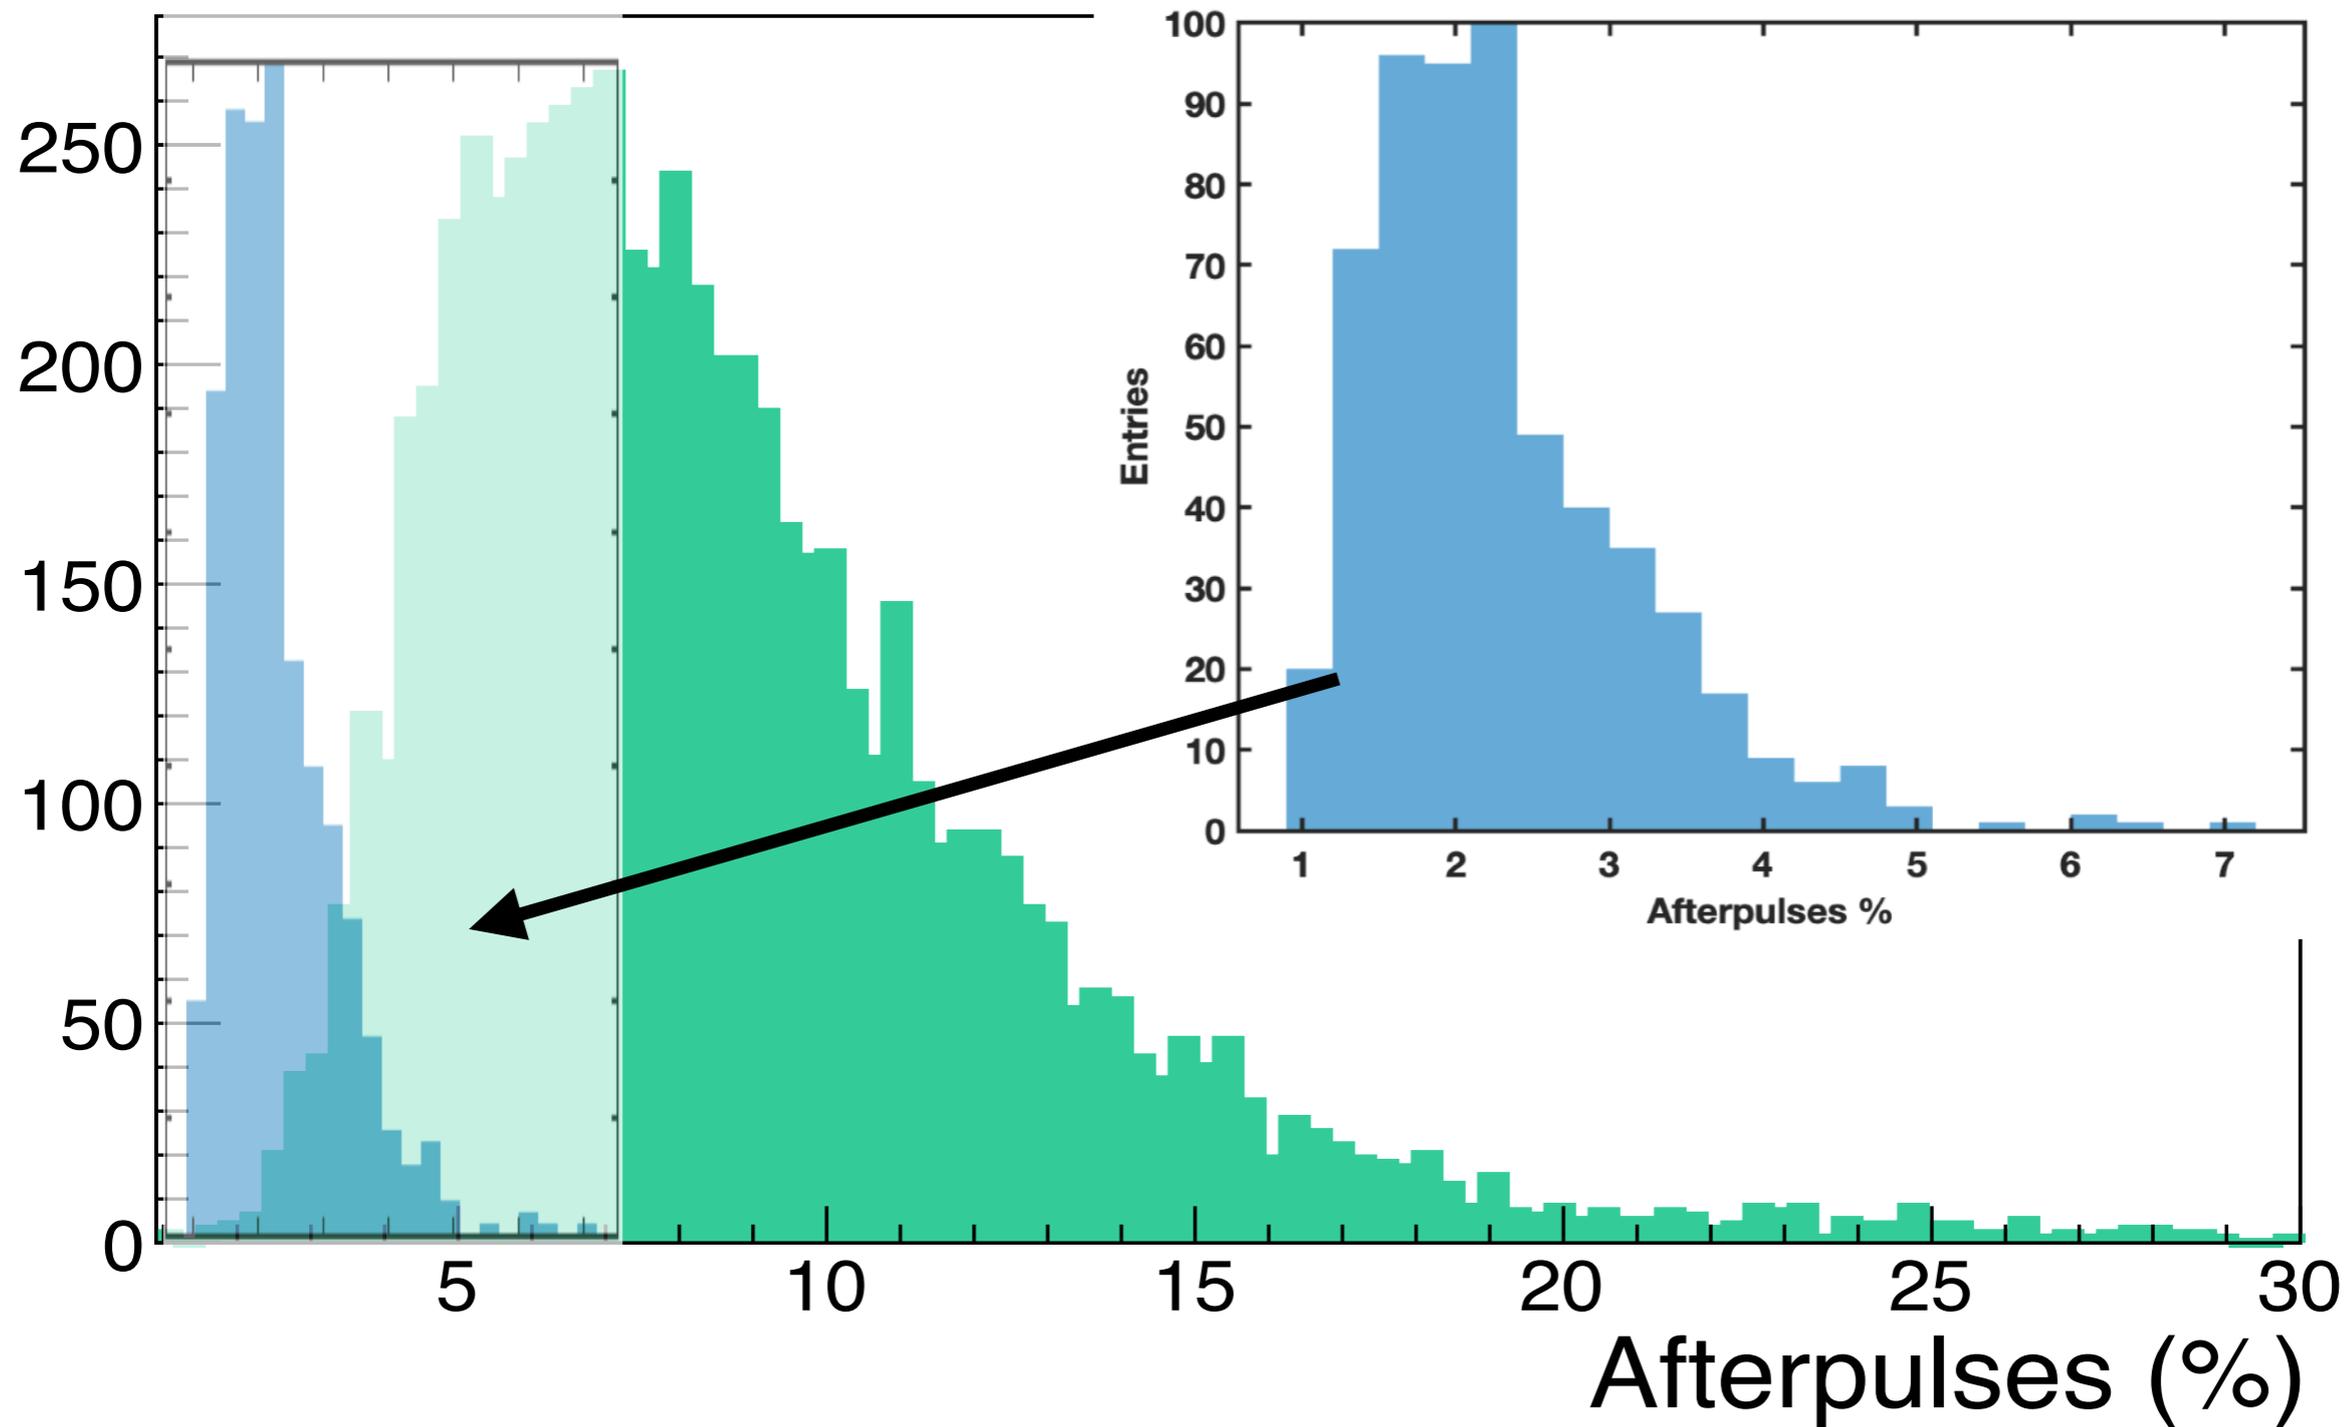


Delayed pulses between 15 ns and 60 ns

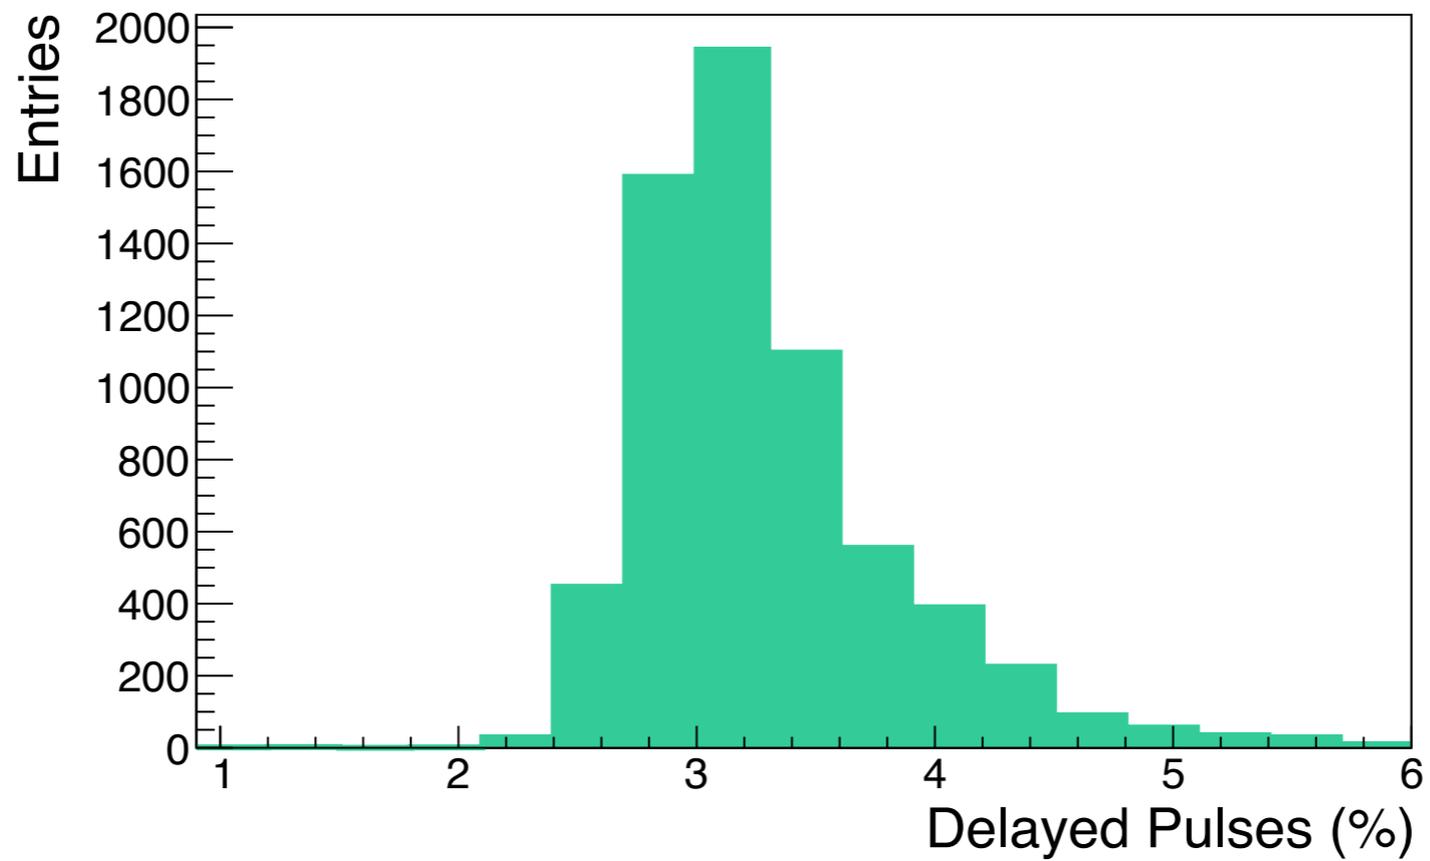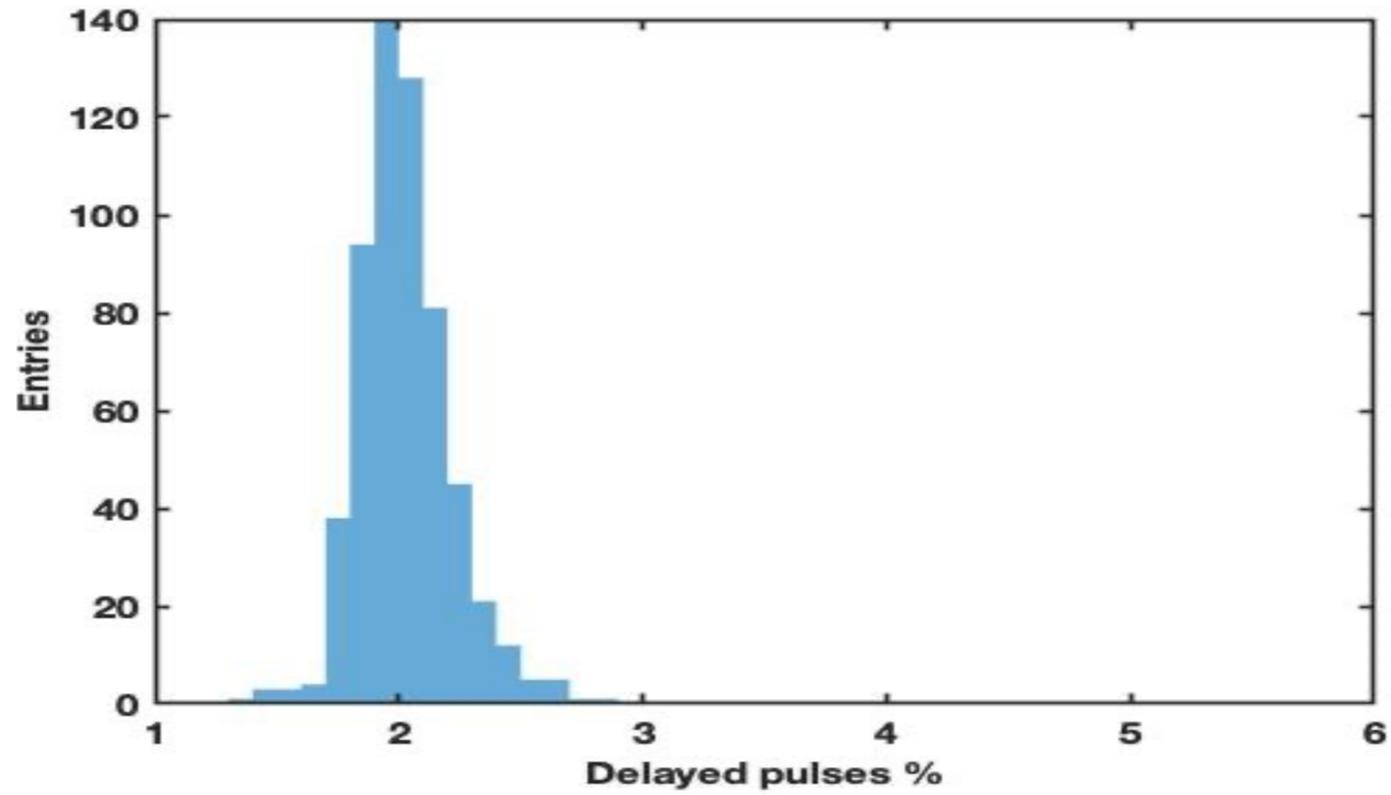


Dark counts rate

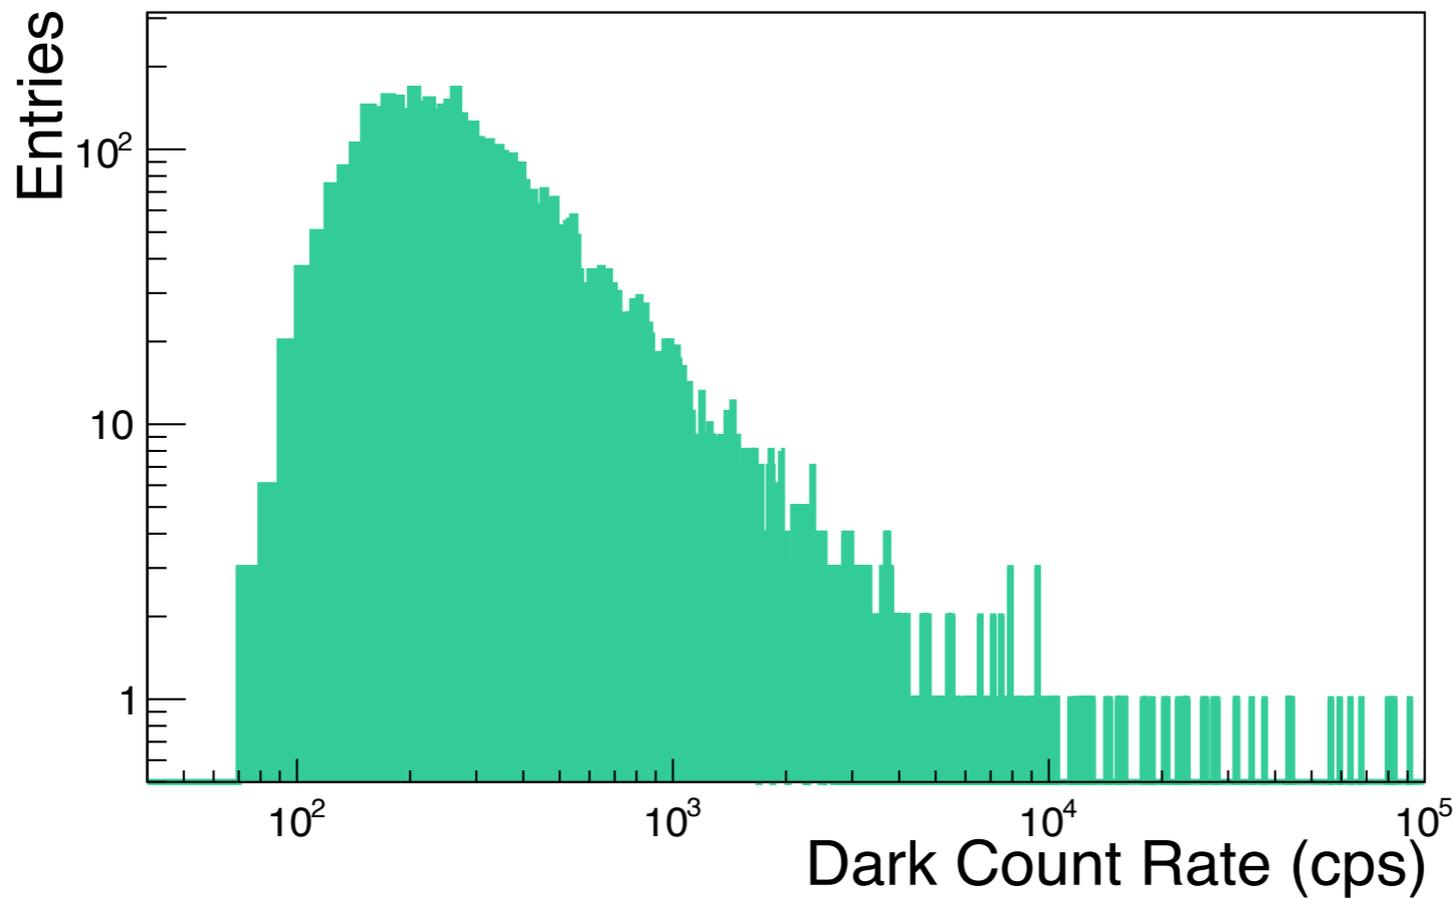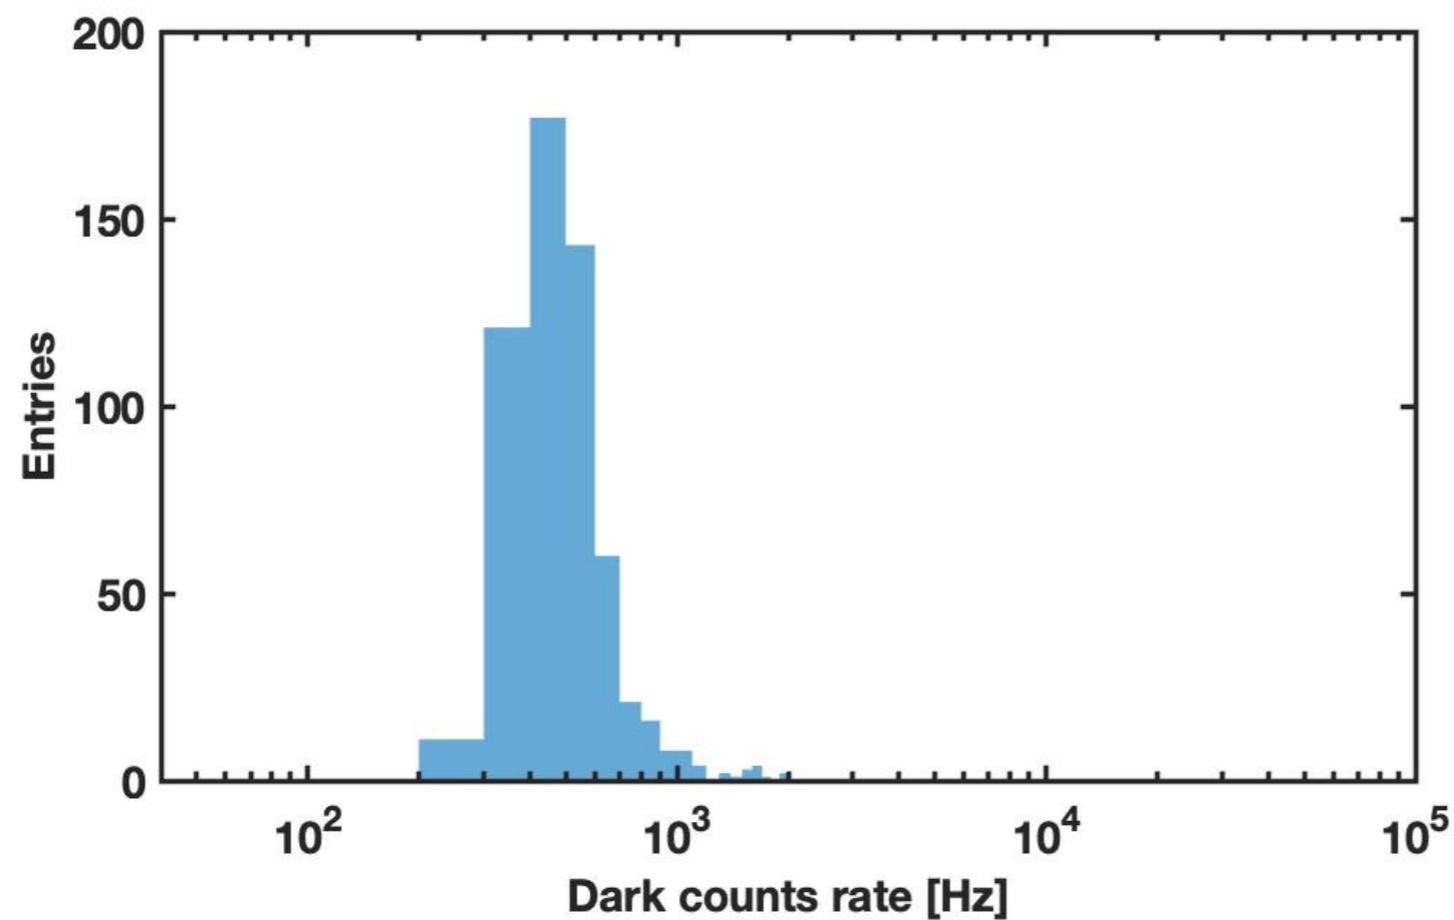

Transit time spread comparison

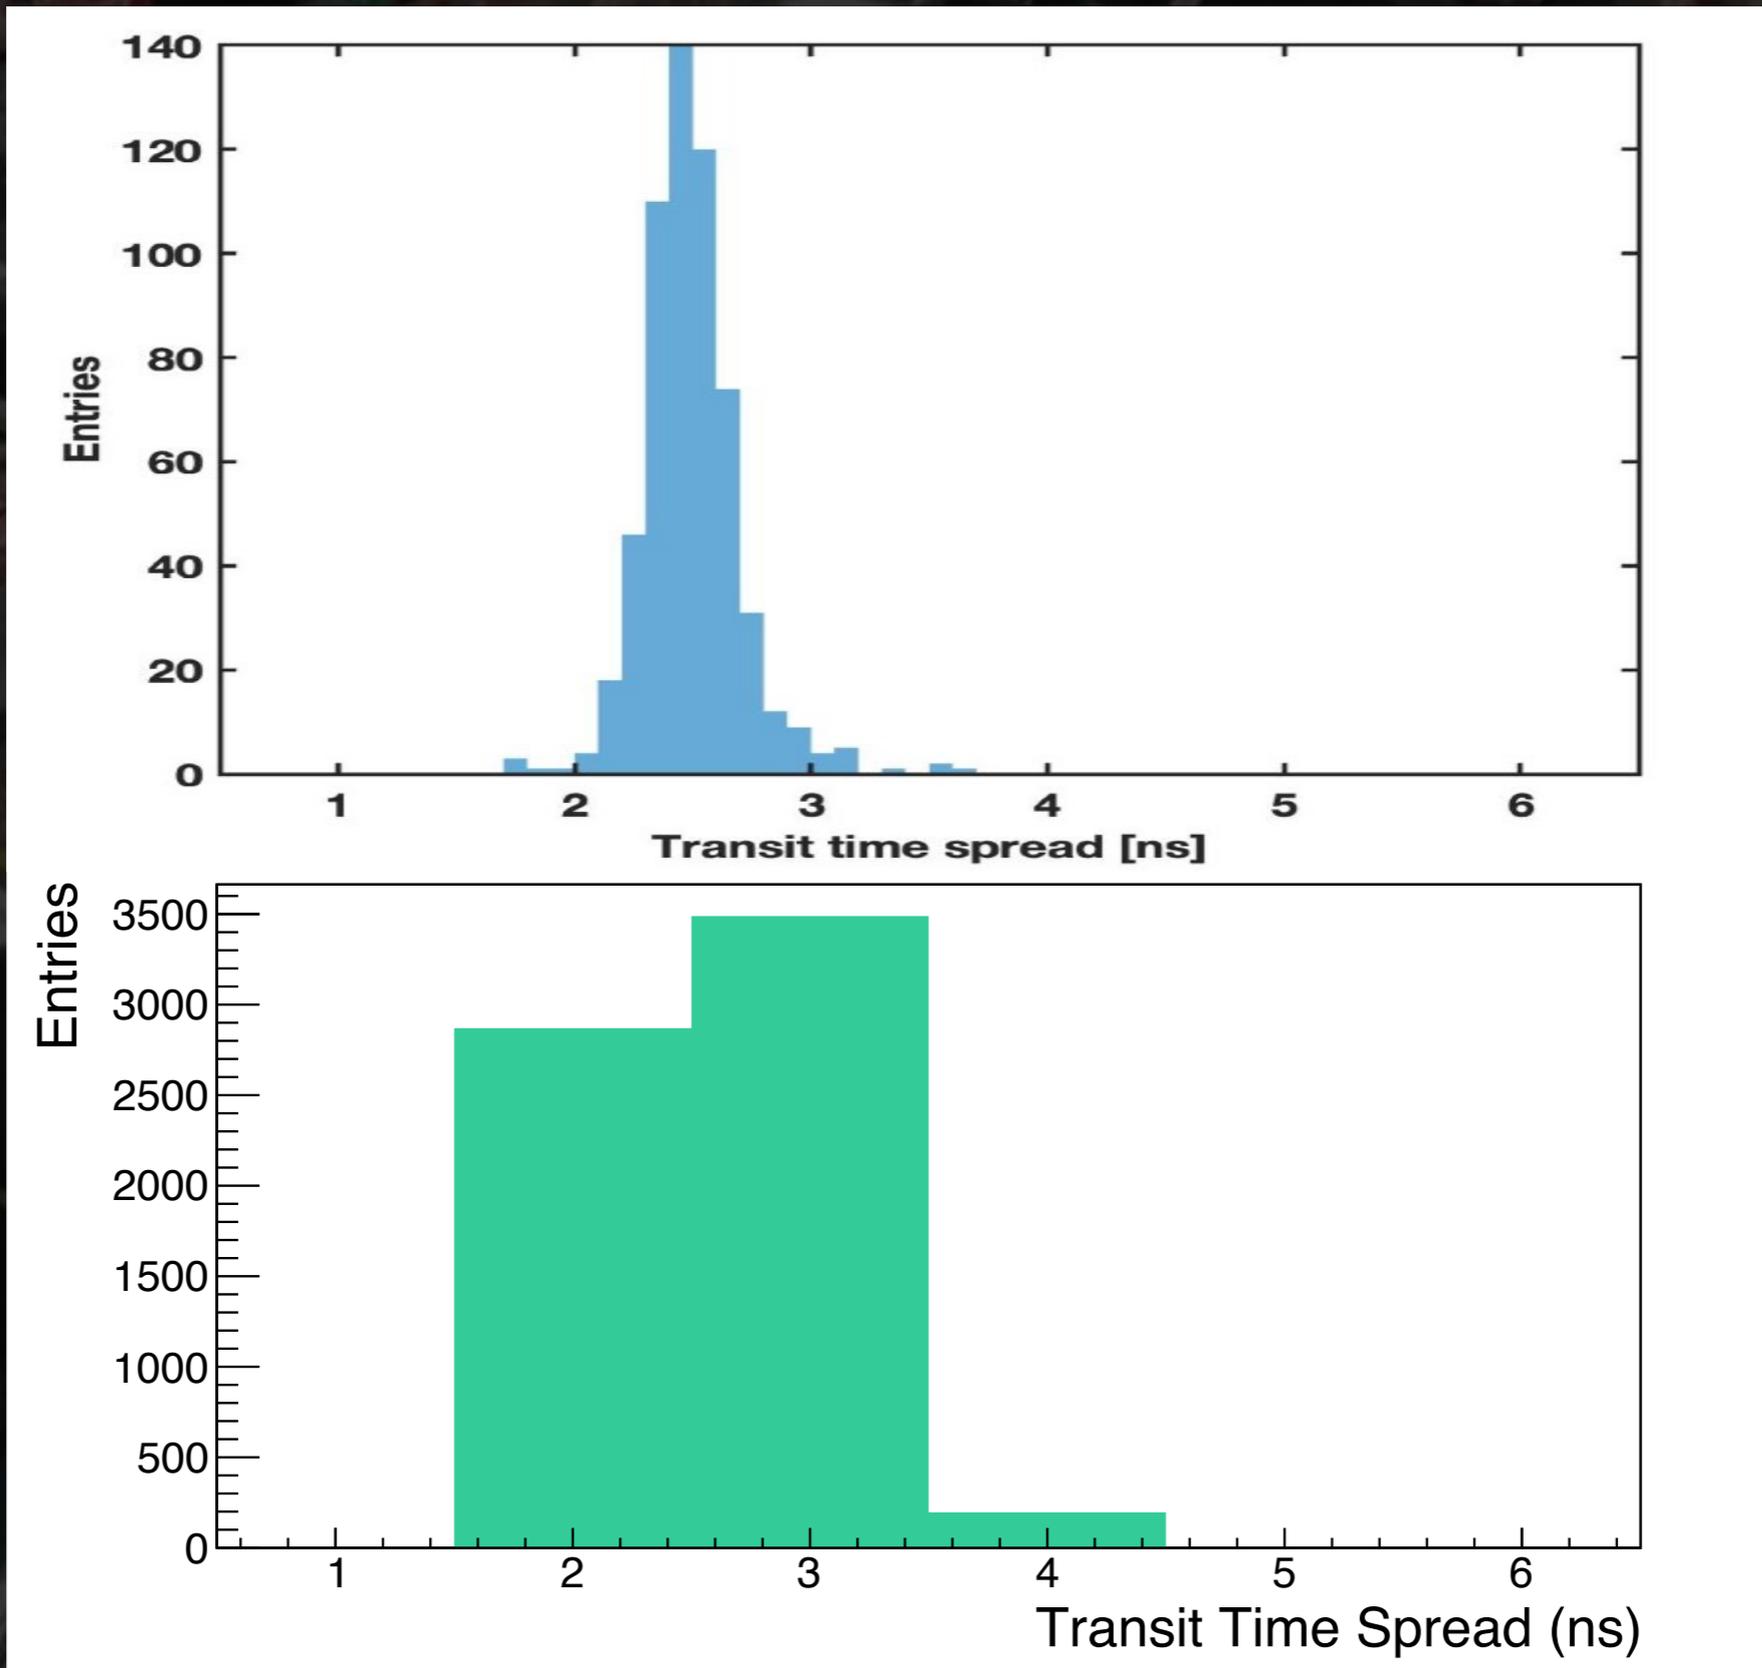

- The new QE setup in Caserta is now fully operative
- New R14374 shows a better spatial QE uniformity and same QE over wavelength
- A comparison between old and new PMT with the same setup is done
- The DarkBox is again operative in Capacity lab for PMTs timing characterisation
- 500 pcs of R14374 PMTs have been measured showing far better timing properties

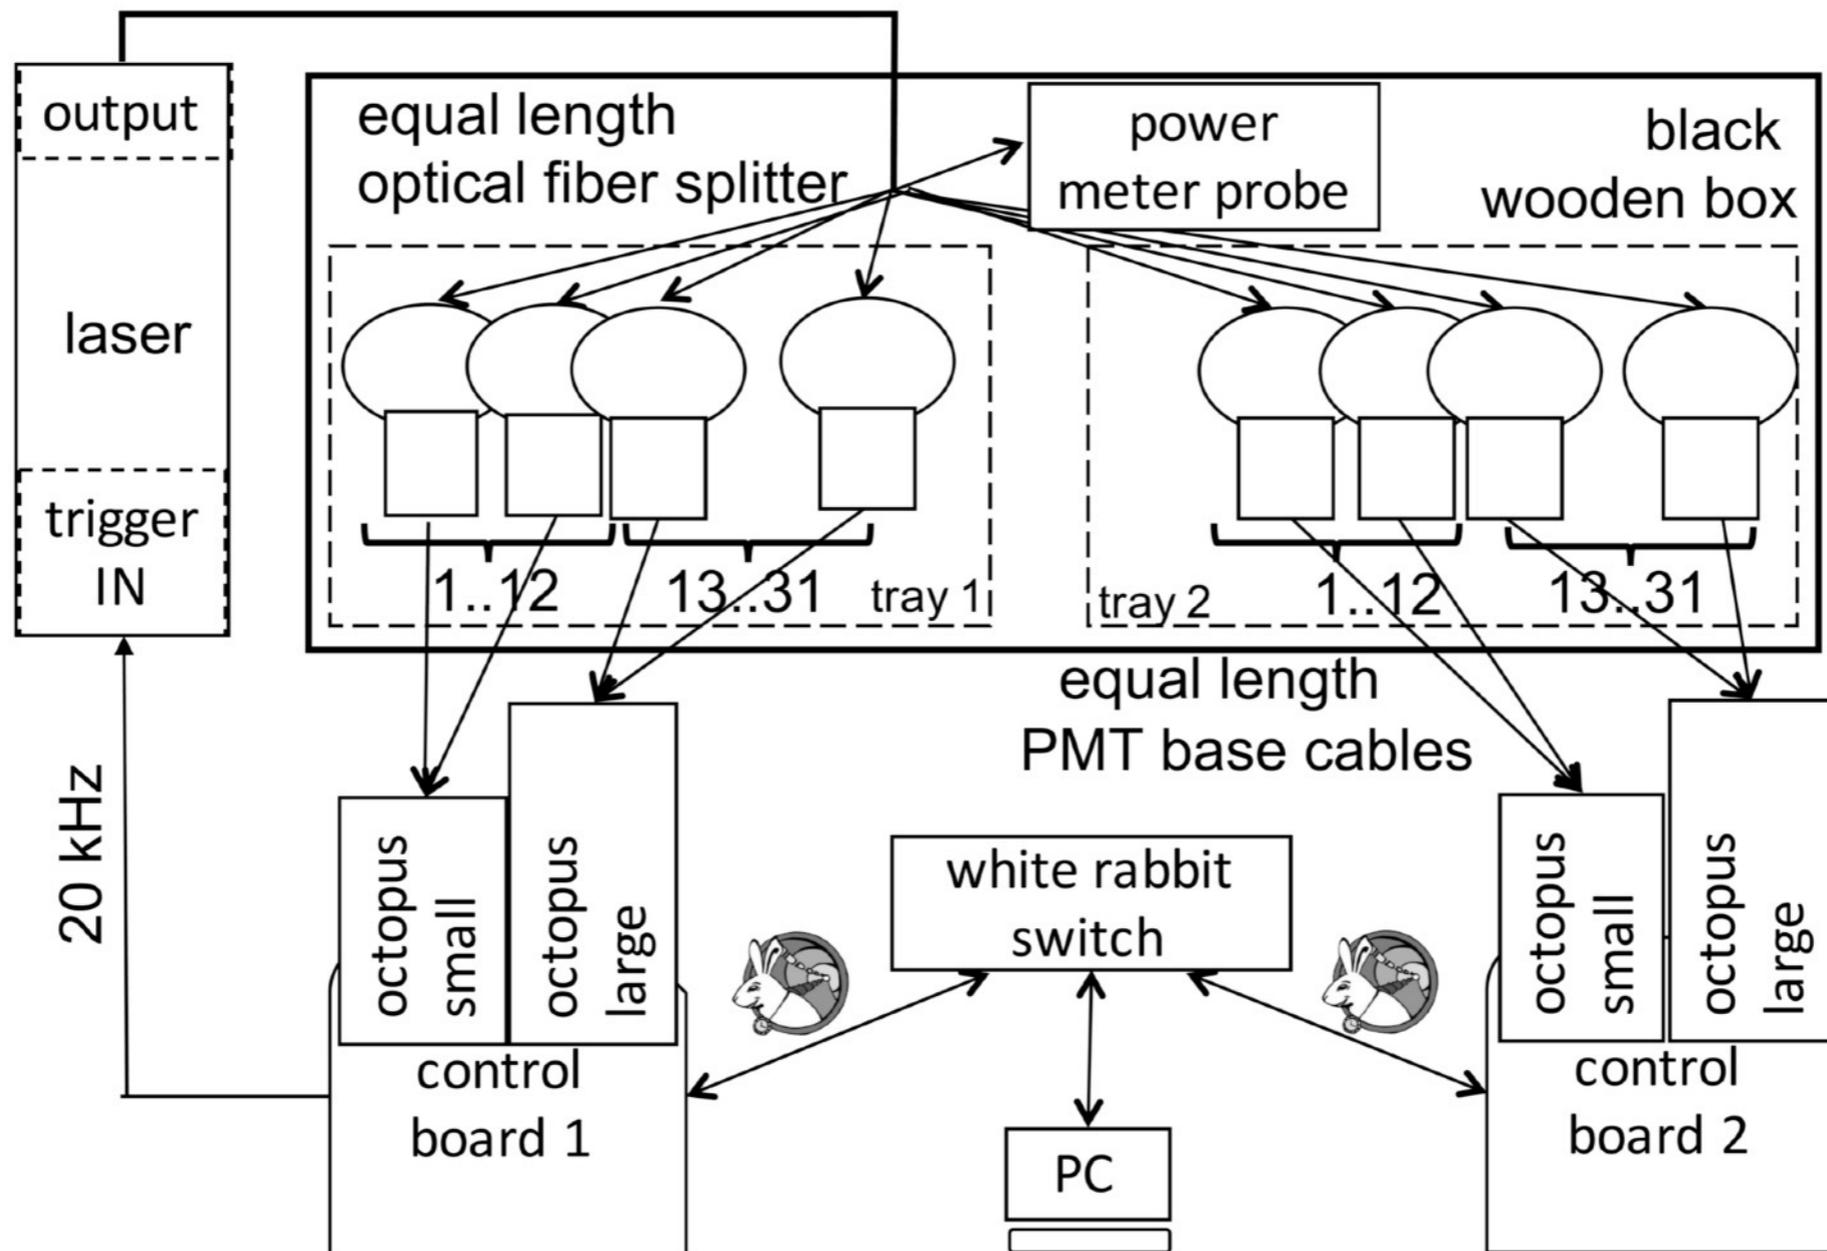

M.C. Mollo et al.

The Dark Box instrument for fast automatic testing of the photomultipliers for KM3NeT
Volume 236 - The 34th International Cosmic Ray Conference (ICRC2015)

Radial variations vs wavelength

