


BCO-counter bug

E.P.


MEG - Telescope interface

- BCO clock signal (counter latched)
- Start RUN (counter reset)
- Unix Time of the event

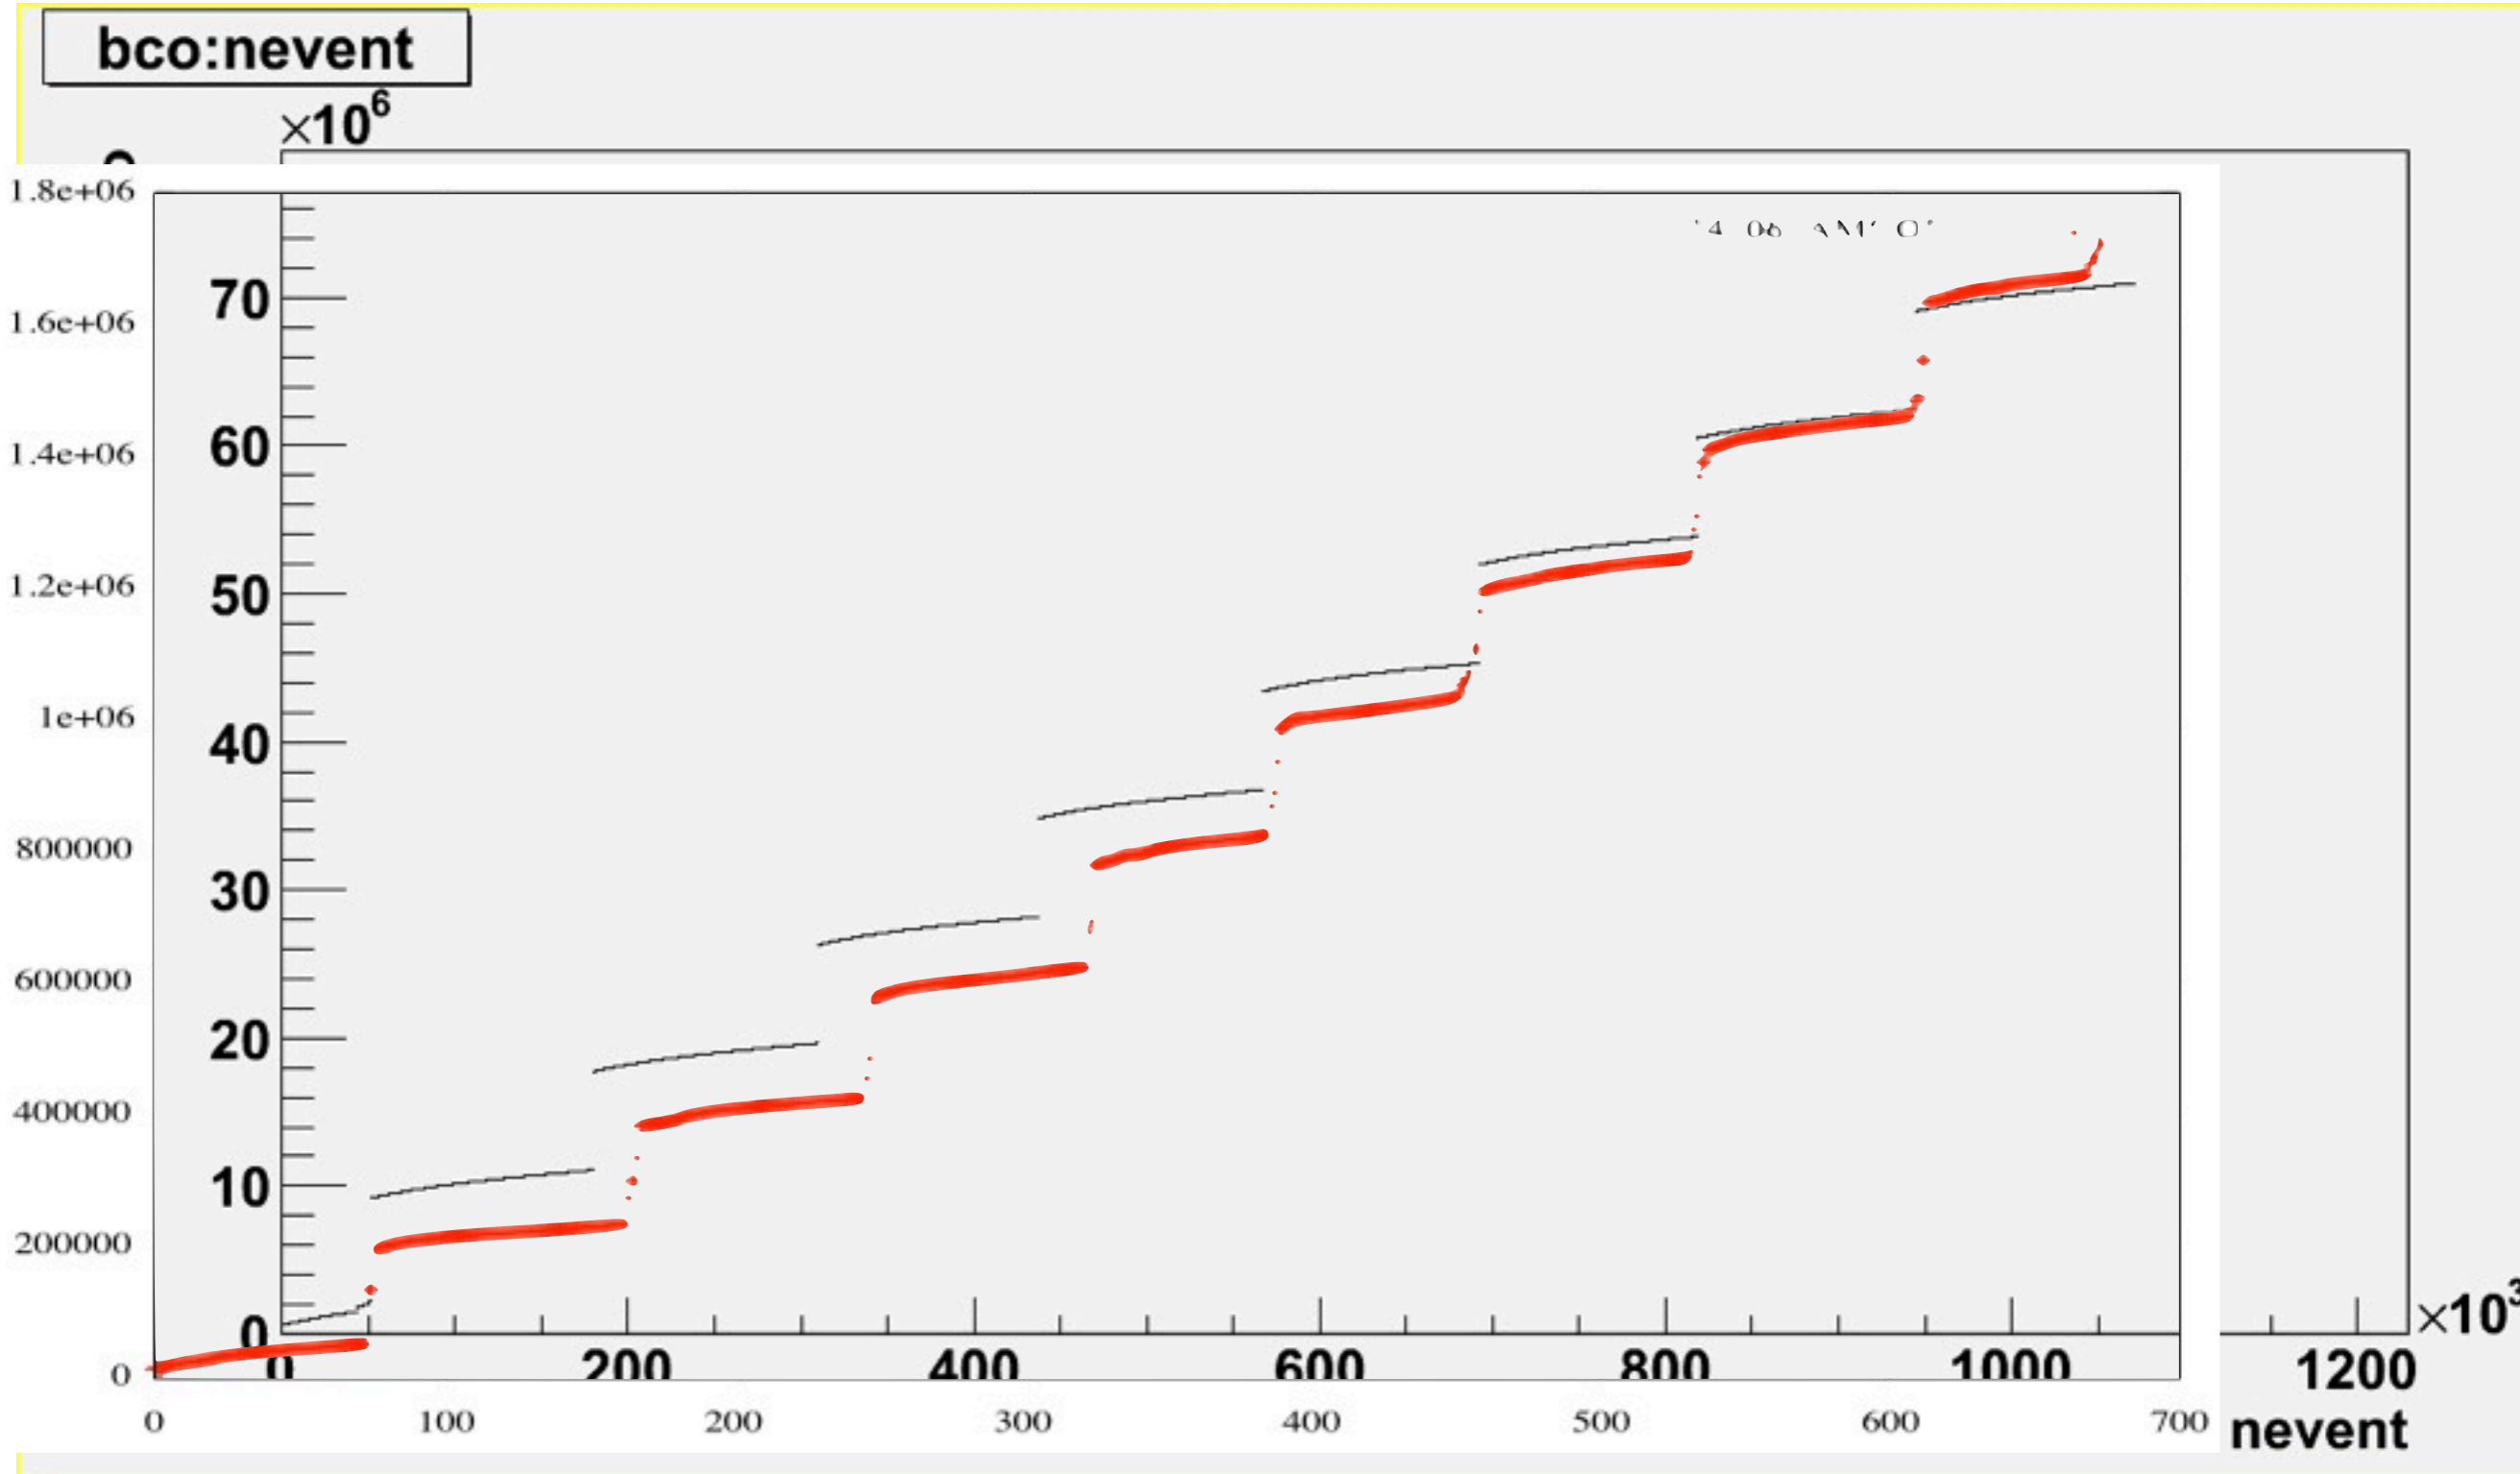

A typical run

D_bco

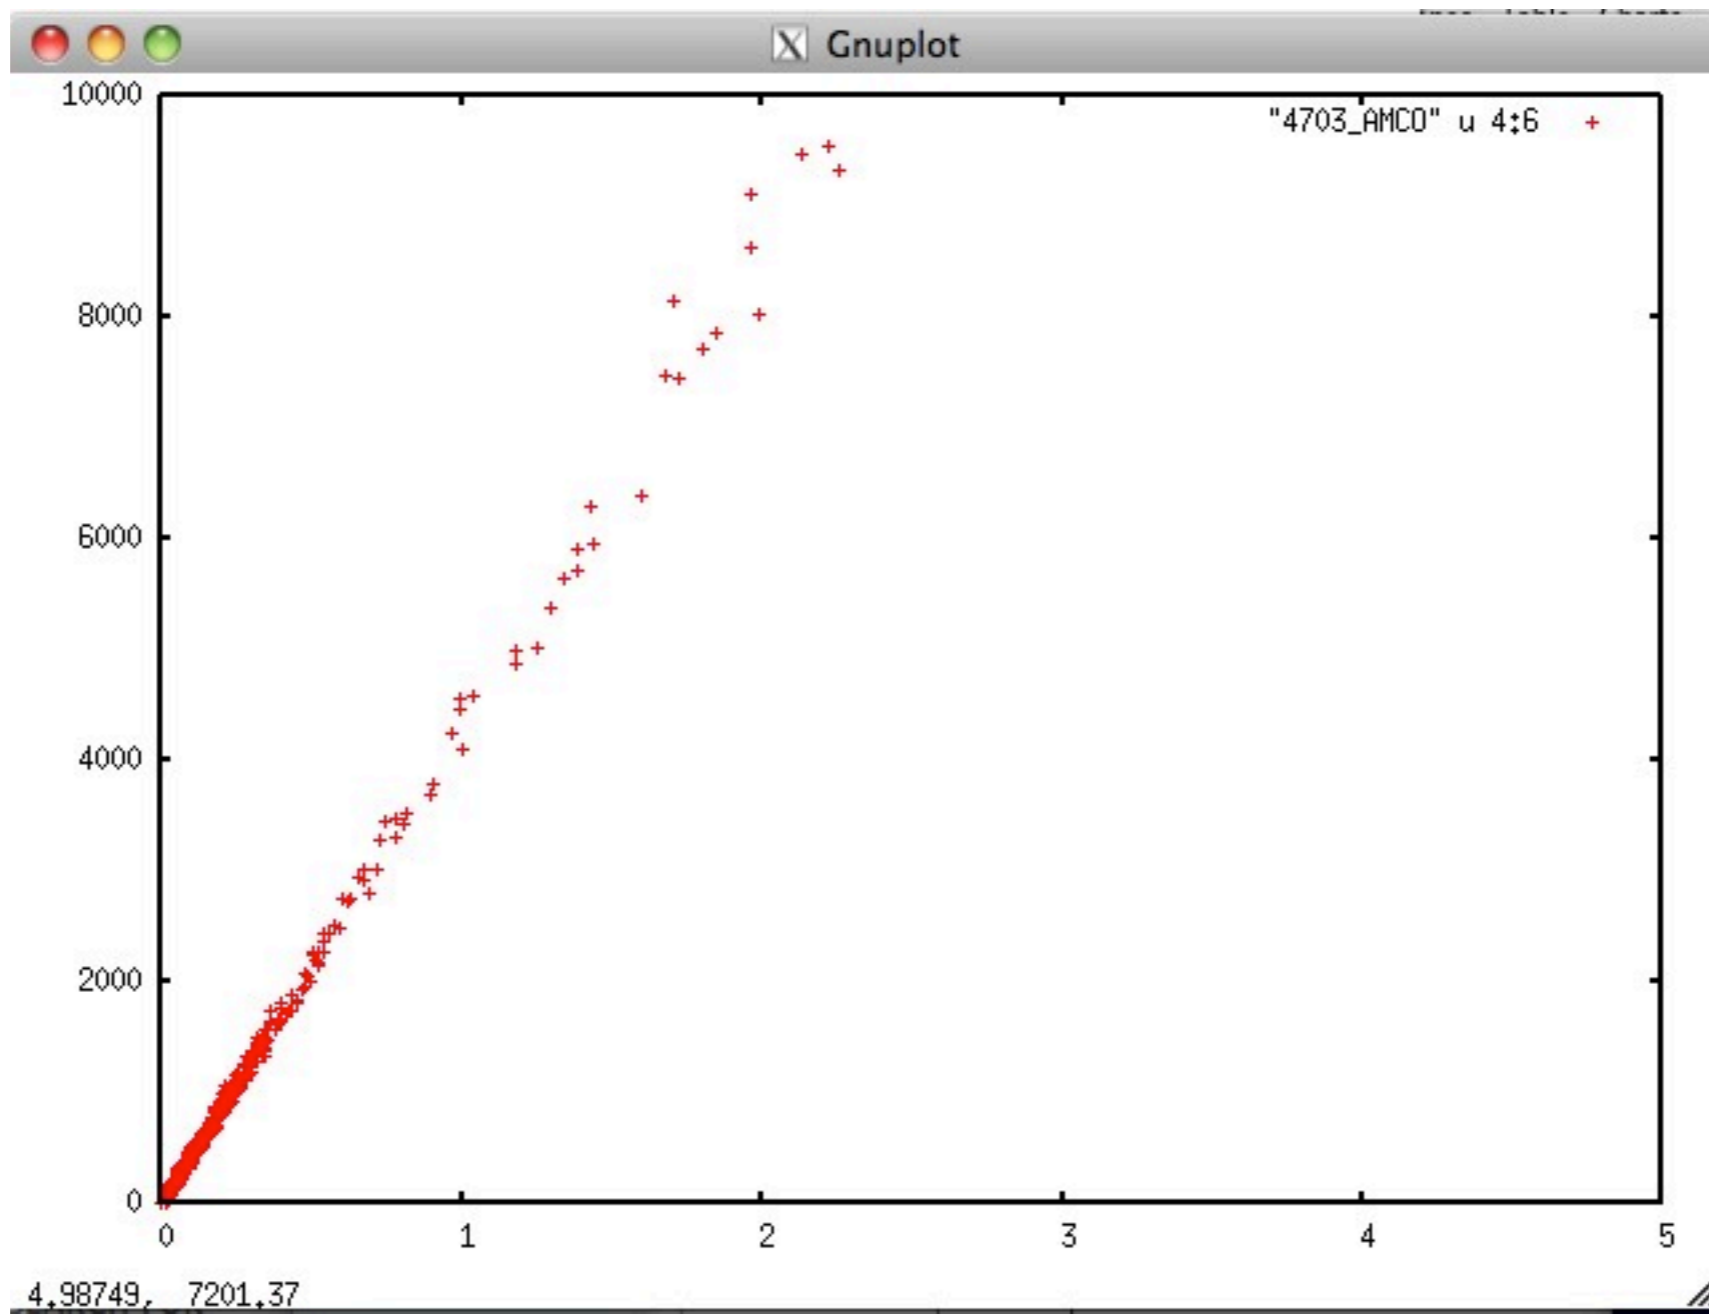

Dt (sec)

BCO bug consequences

- The telescope \leftrightarrow MEG synchronization is based on the BCO counter
- the BCO counter on the MEG boards is flacky (random resets on a few runs)